

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 08/08/2022

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 22190

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:58
INTERNAL STANDARD	VERIFIED	13:59
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	13:59
BLANK TEST	0.00	14:00
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	14:00
BLANK TEST	0.00	14:01
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	14:01
BLANK TEST	0.00	14:02

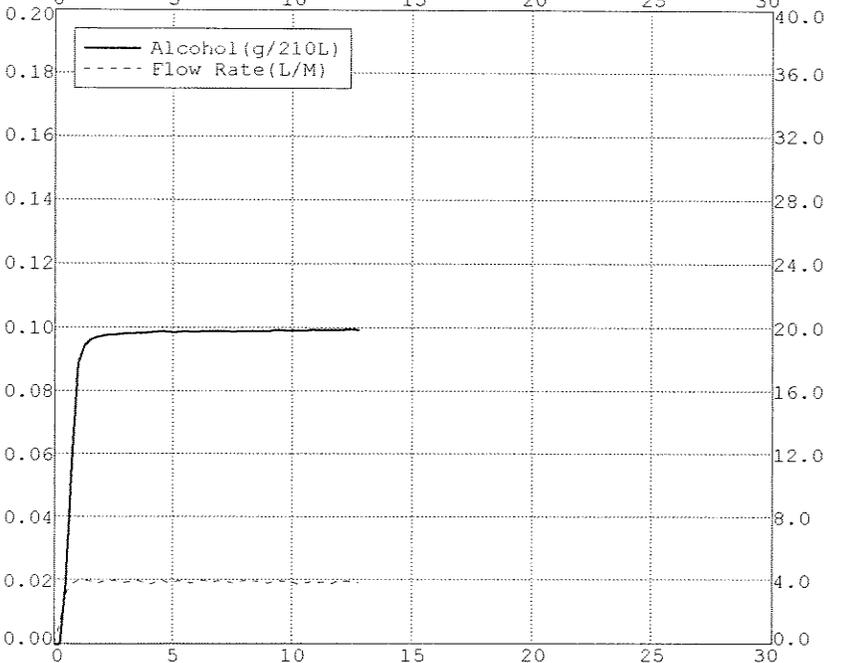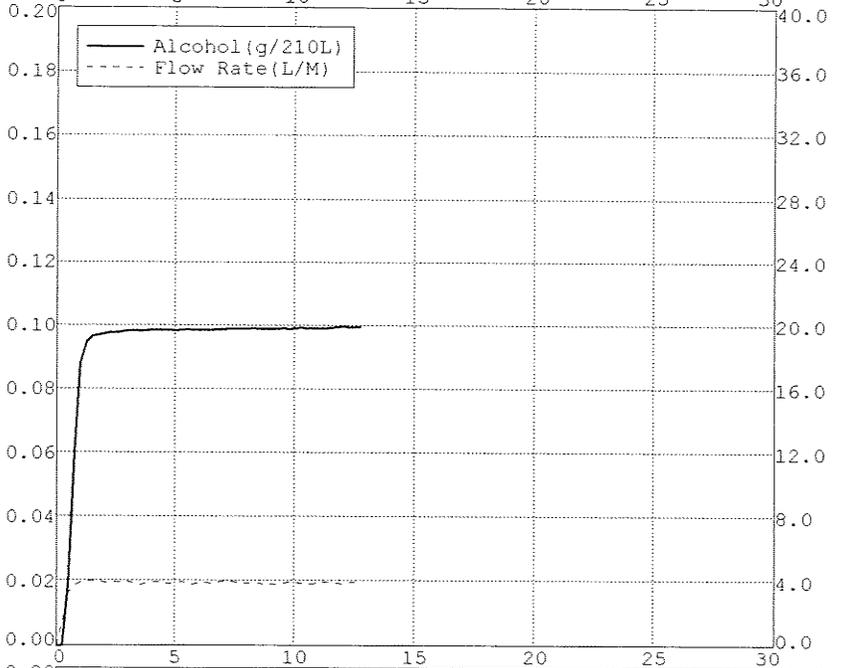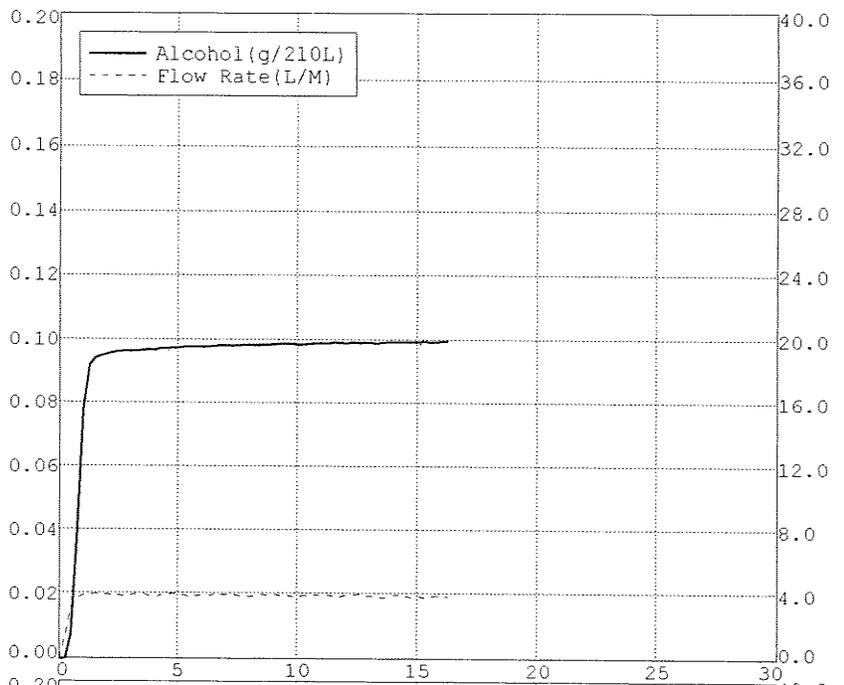

*Sgt. C. B. Geisler*