

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 09/16/2022

OPERATOR NAME:  
J RIEHL  
Permit #: 47503  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 22190

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:42
INTERNAL STANDARD	VERIFIED	00:42
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:43
BLANK TEST	0.00	00:44
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:44
BLANK TEST	0.00	00:45
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:45
BLANK TEST	0.00	00:46

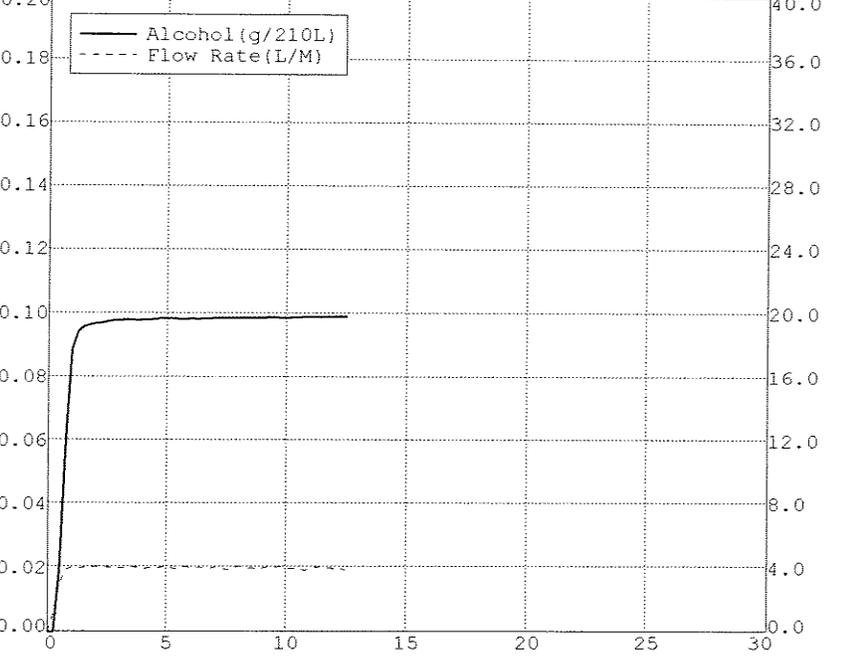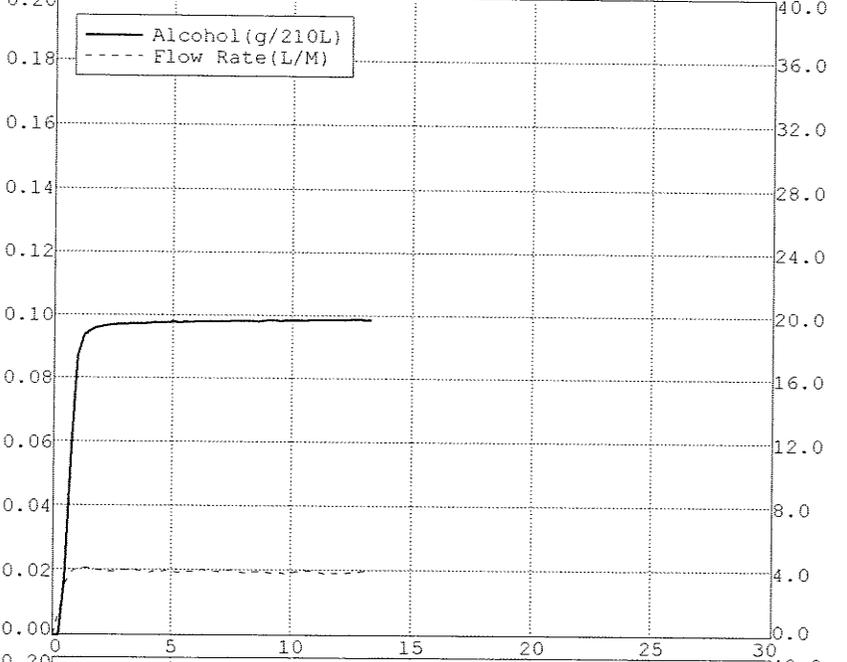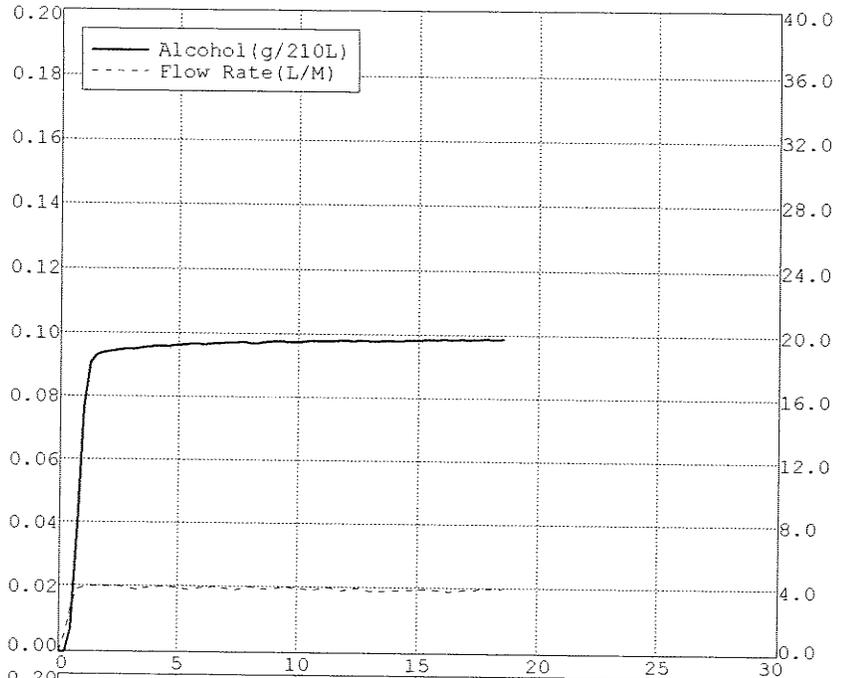

*[Handwritten signature]*  
#1820