

SOLUTION CHANGE



WARREN CO.
 SHERIFF'S OFFICE
 DATAMASTER dmt: 105208

Date: 11/01/2022

OPERATOR NAME:
 CHARLES B GEISLER
 Permit #: 33757
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 22260

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:43
INTERNAL STANDARD	VERIFIED	13:43
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	13:44
BLANK TEST	0.00	13:44
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	13:45
BLANK TEST	0.00	13:46
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	13:46
BLANK TEST	0.00	13:47

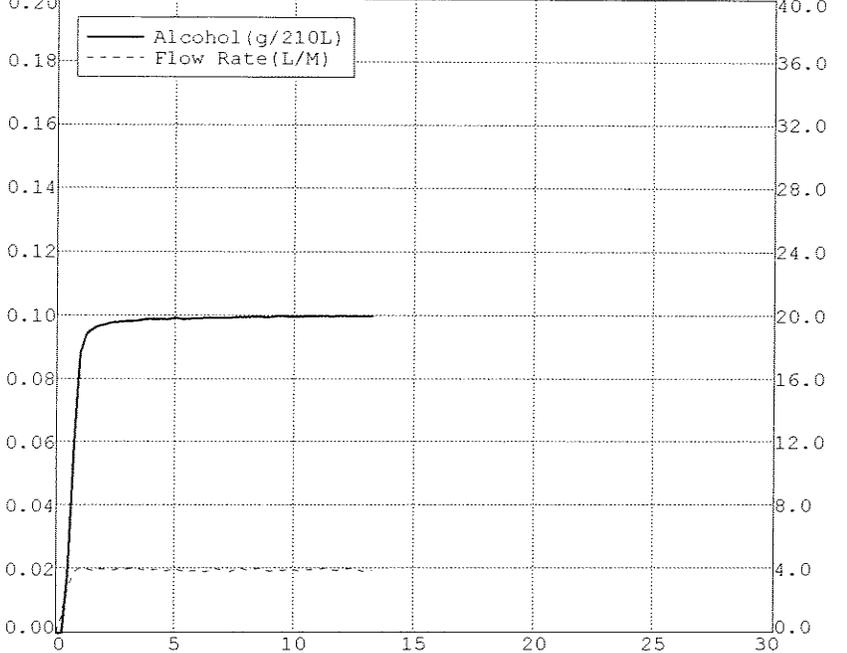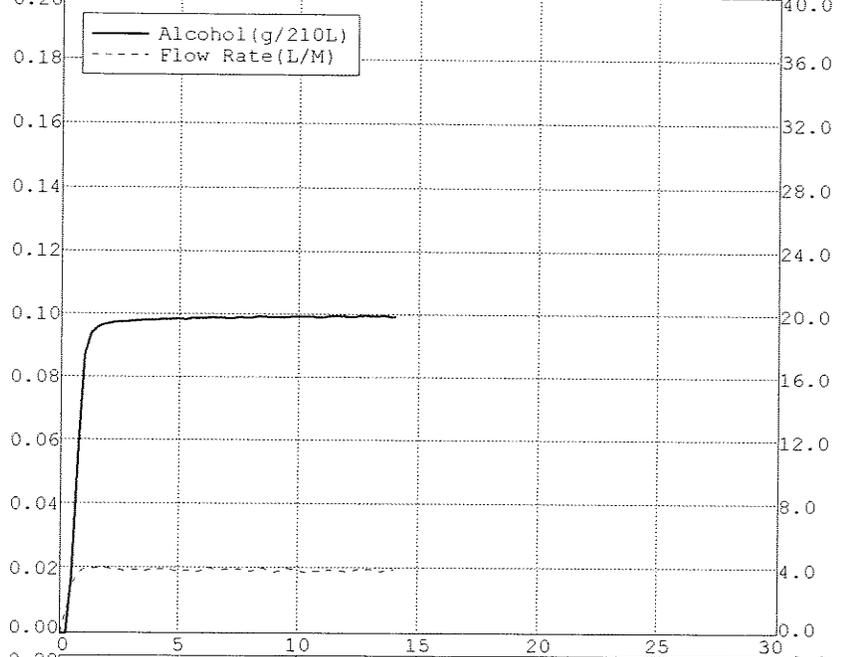

Sp. Chl - B. C. Geisler