

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 11/07/2022

OPERATOR NAME:  
J RIEHL  
Permit #: 47503  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 22260

Nominal = 0.10 g/210L

BLANK TEST	0.00	05:00
INTERNAL STANDARD	VERIFIED	05:00
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	05:00
BLANK TEST	0.00	05:01
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	05:02
BLANK TEST	0.00	05:02
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	05:03
BLANK TEST	0.00	05:04

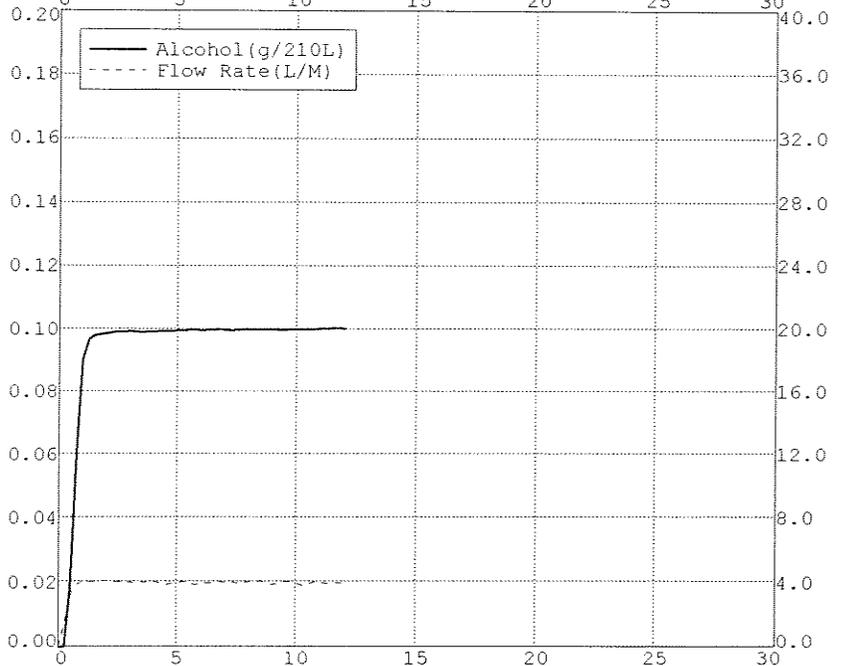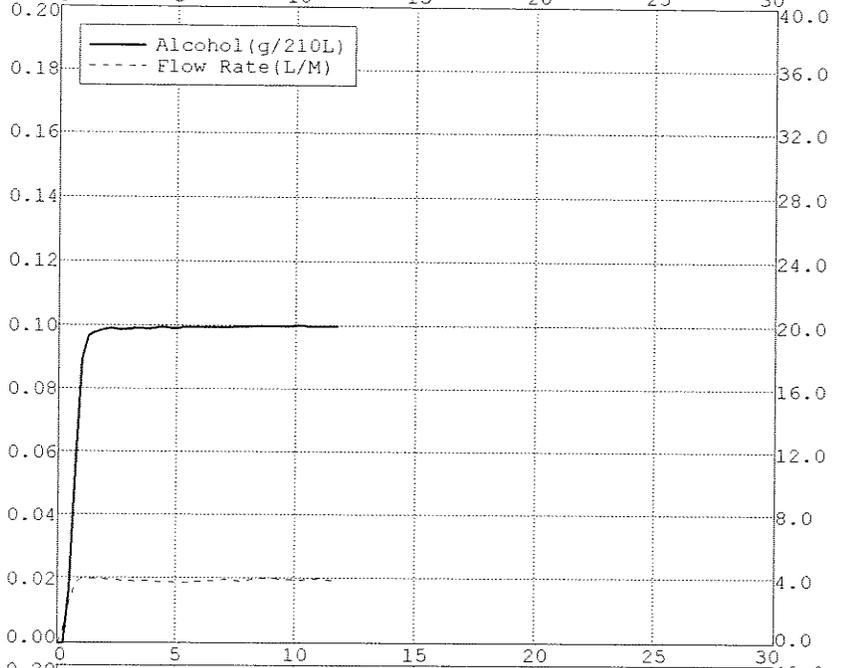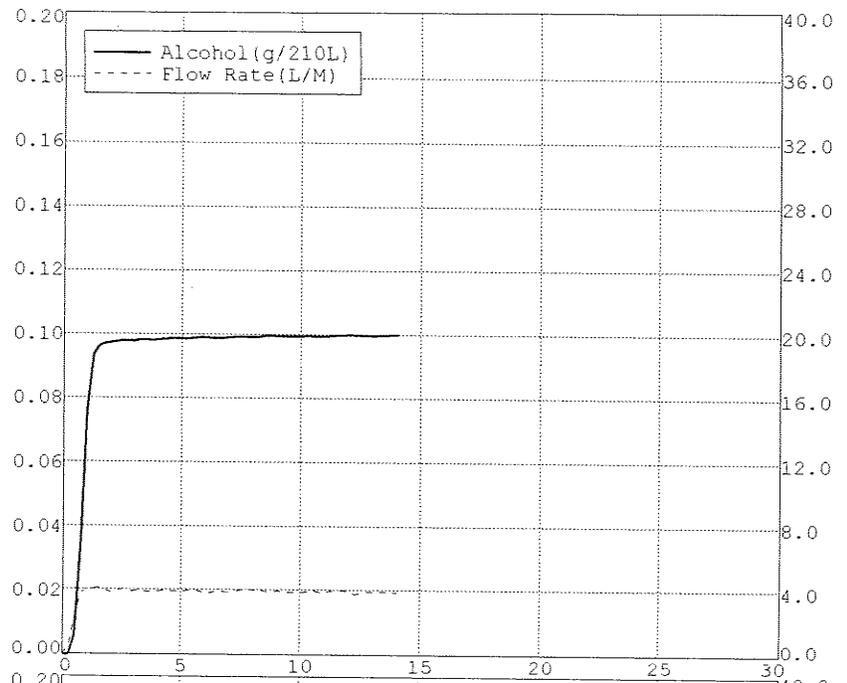

#820