

SOLUTION CHANGE




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 12/01/2022

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 22390

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:14
INTERNAL STANDARD	VERIFIED	13:14
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	13:15
BLANK TEST	0.00	13:15
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	13:16
BLANK TEST	0.00	13:17
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	13:17
BLANK TEST	0.00	13:18

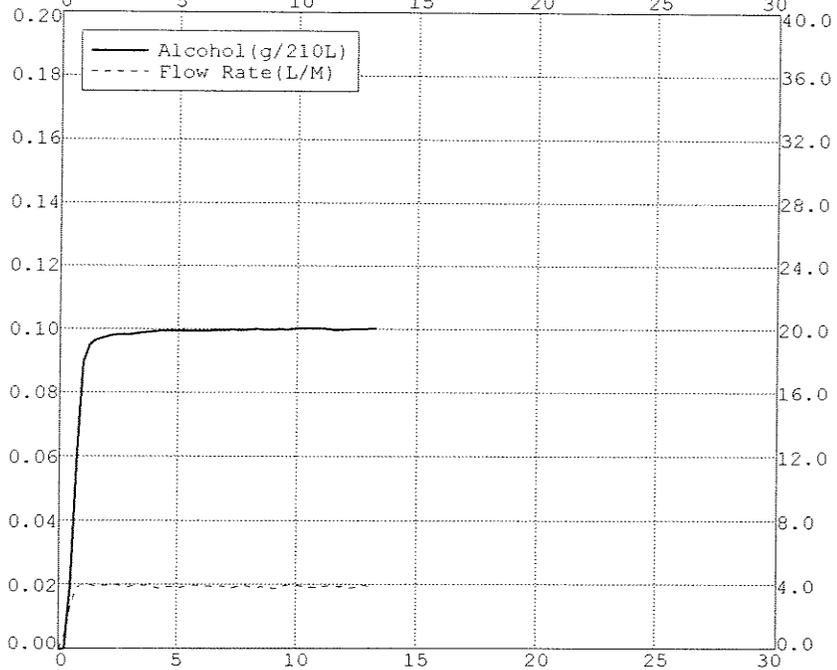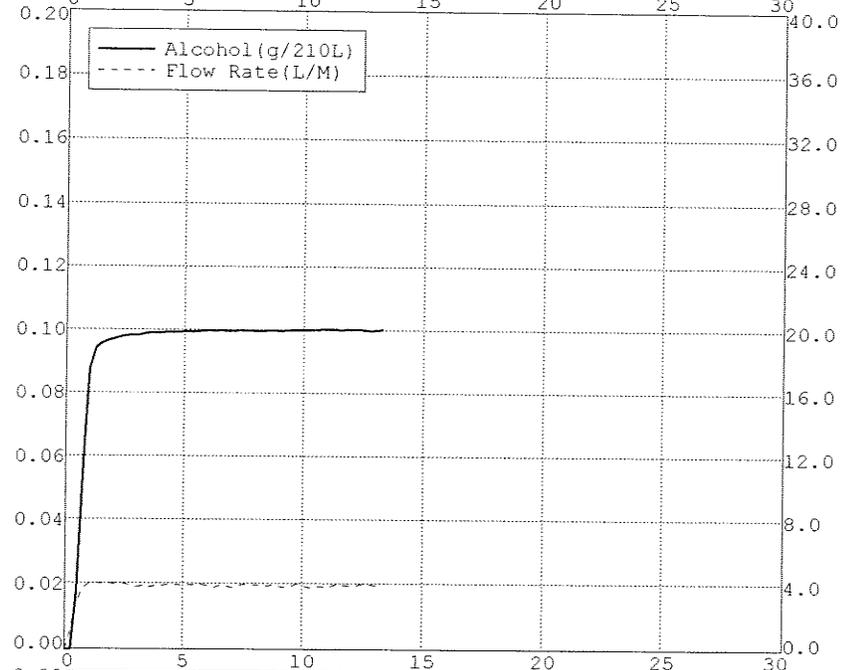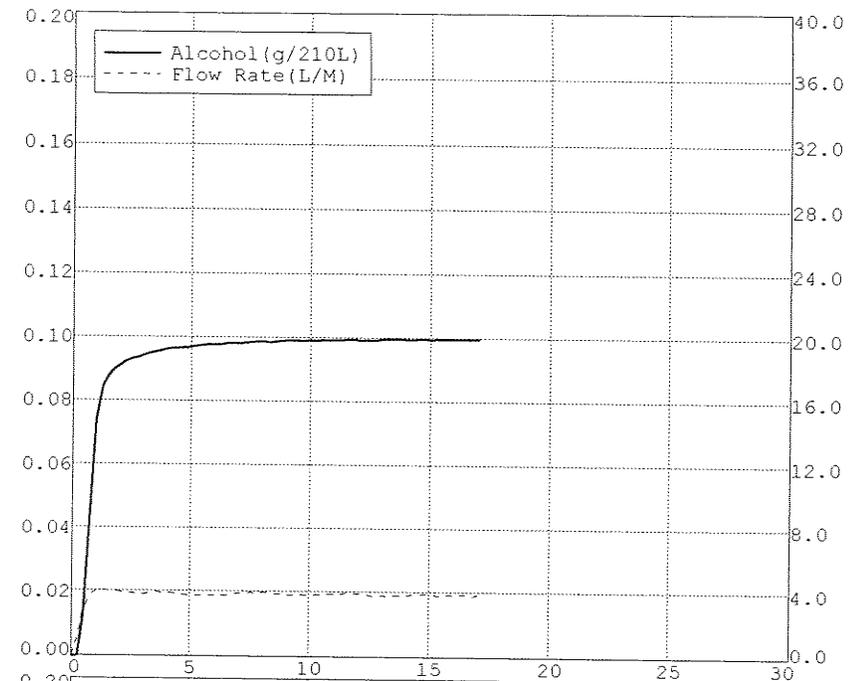

*Charles B. Geisler* #241