

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 12/26/2022

OPERATOR NAME:
SEAN T SMITH
Permit #: 46227
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 22390

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:09
INTERNAL STANDARD	VERIFIED	09:09
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	09:10
BLANK TEST	0.00	09:11
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	09:11
BLANK TEST	0.00	09:12
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	09:12
BLANK TEST	0.00	09:13

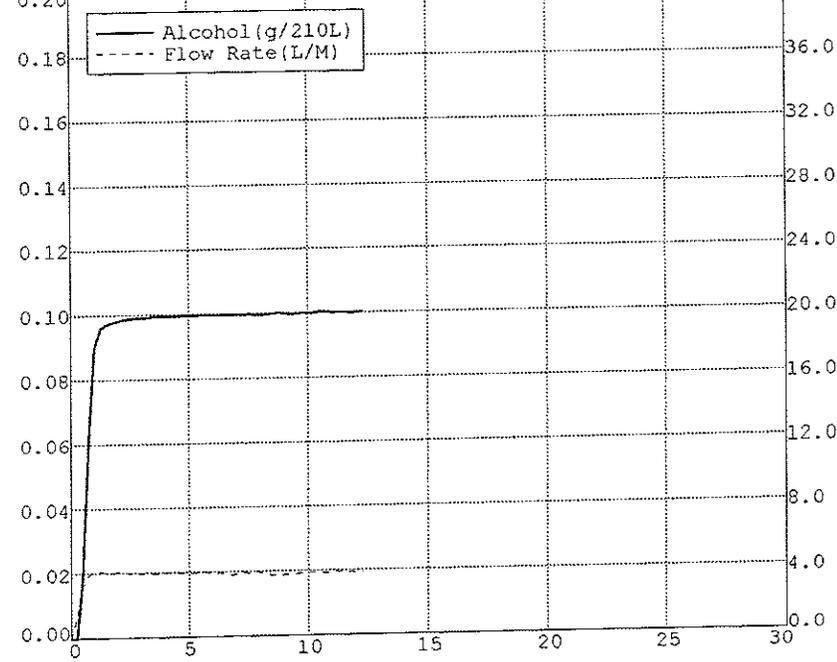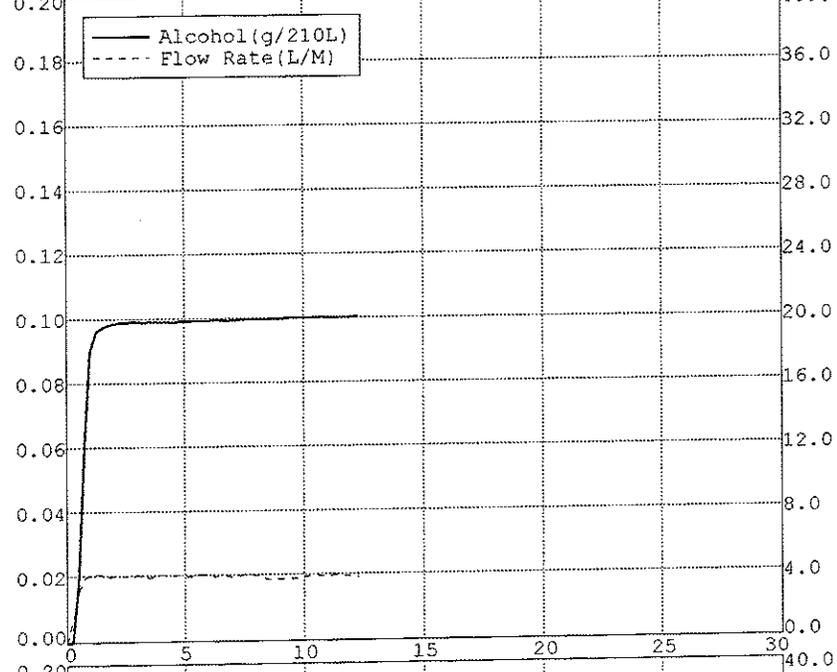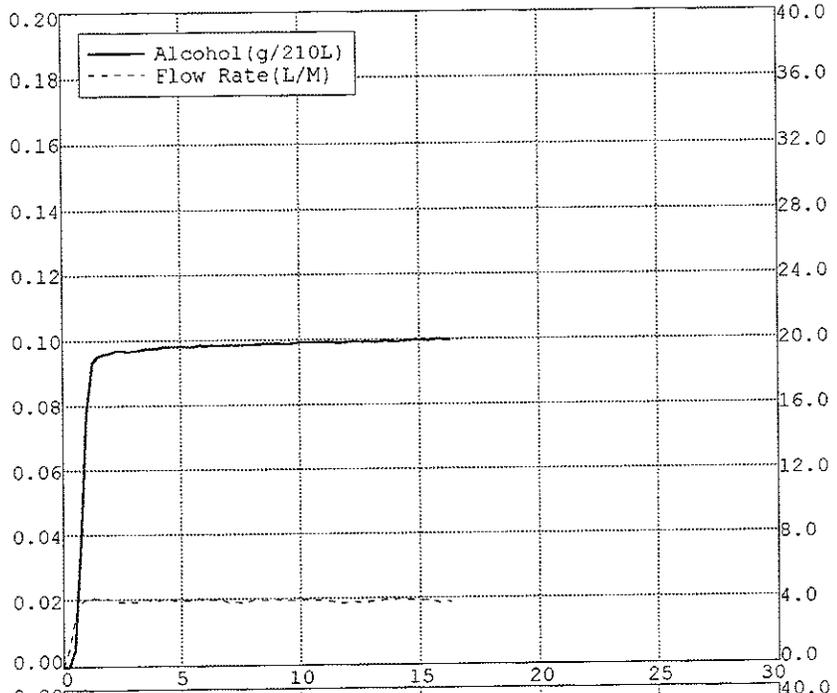

[Handwritten signature] 815