

SOLUTION CHANGE




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 01/01/2022

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 21390

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:51
INTERNAL STANDARD	VERIFIED	15:51
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	15:52
BLANK TEST	0.00	15:53
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	15:53
BLANK TEST	0.00	15:54
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	15:54
BLANK TEST	0.00	15:55

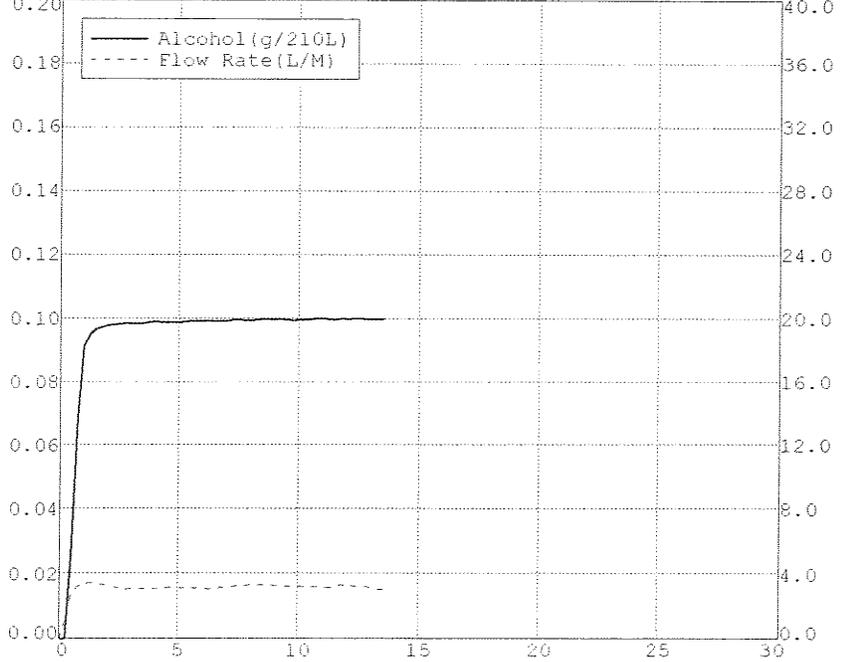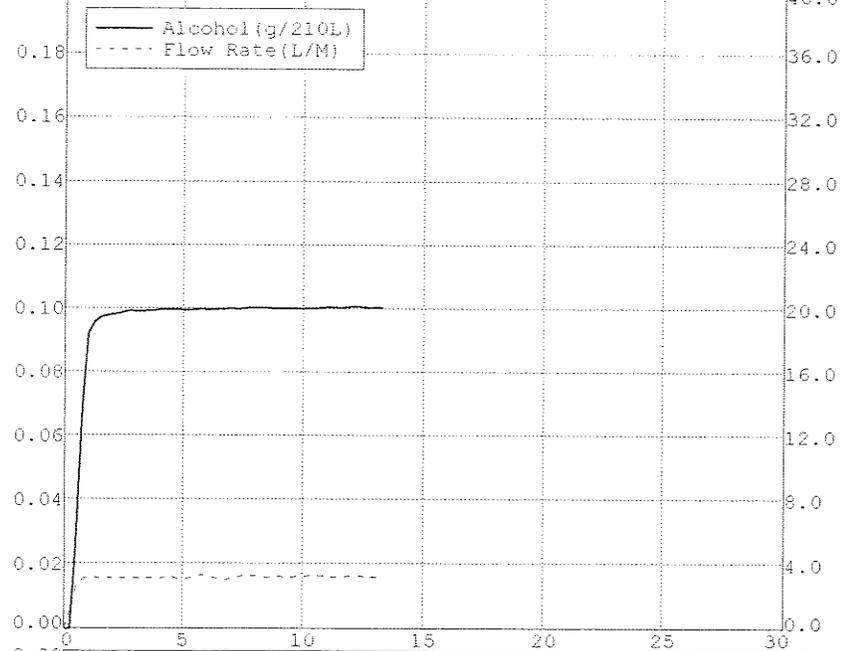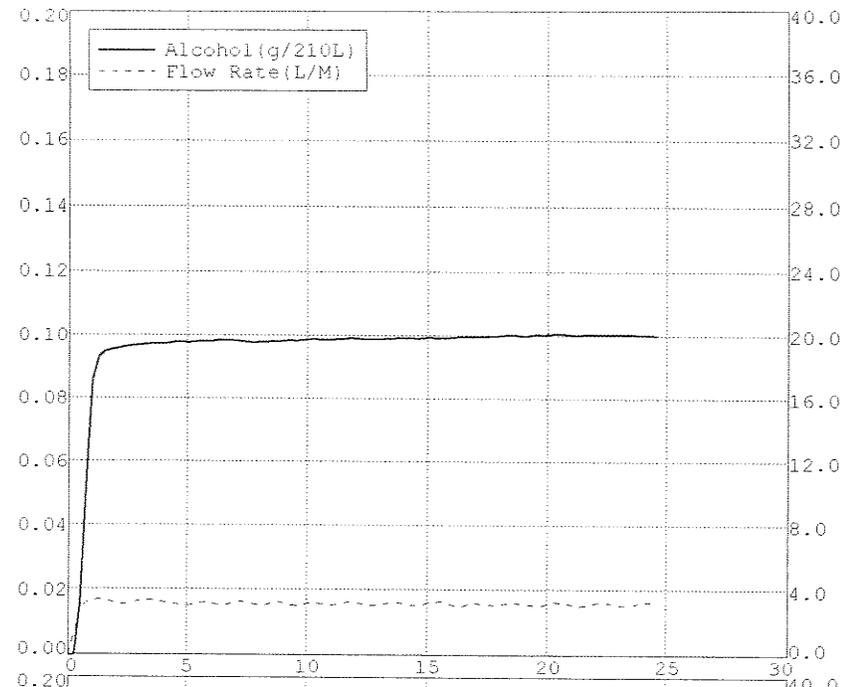

Sgt. Charles B. Geisler #22