

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 01/16/2022

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 21390

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:27
INTERNAL STANDARD	VERIFIED	15:28
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	15:28
BLANK TEST	0.00	15:29
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	15:29
BLANK TEST	0.00	15:30
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	15:30
BLANK TEST	0.00	15:31

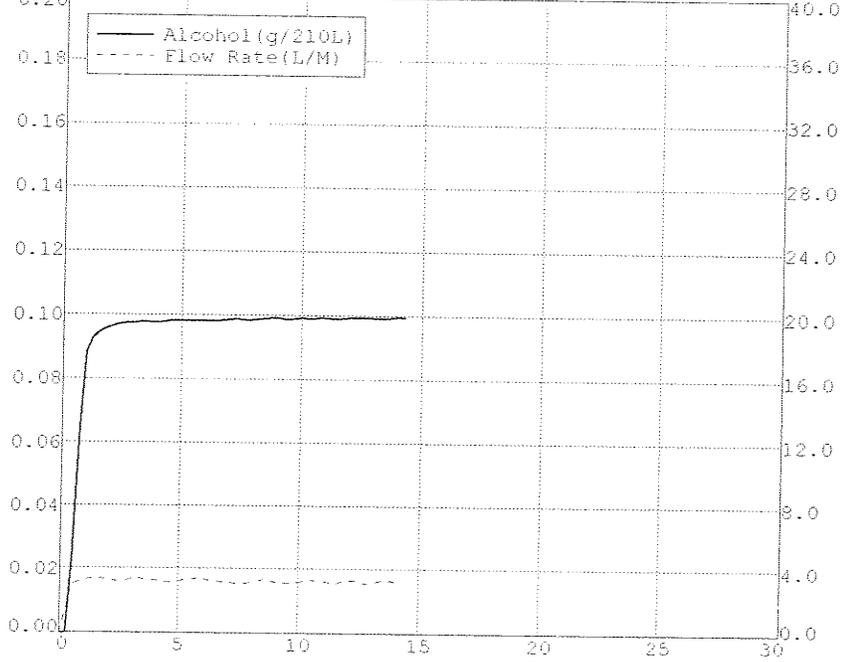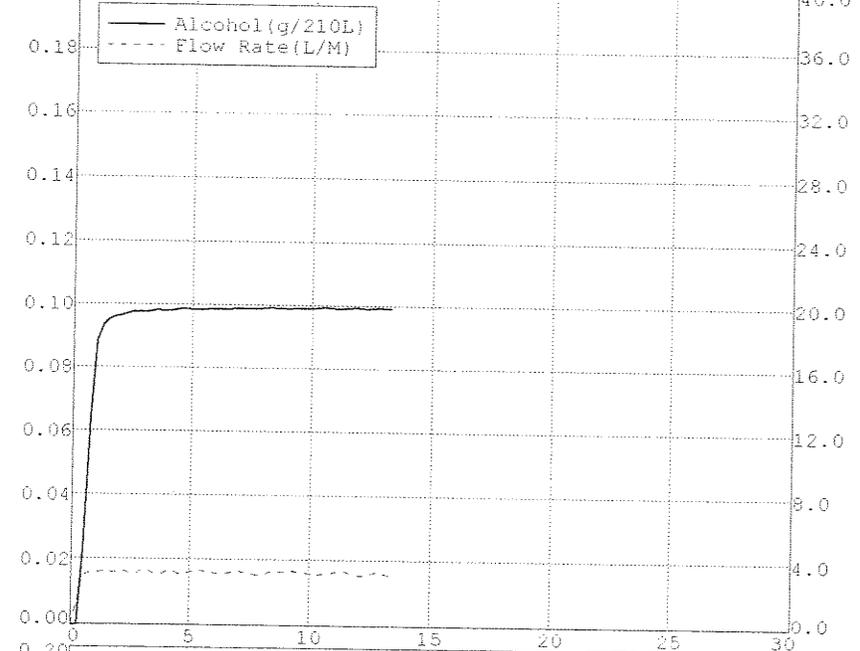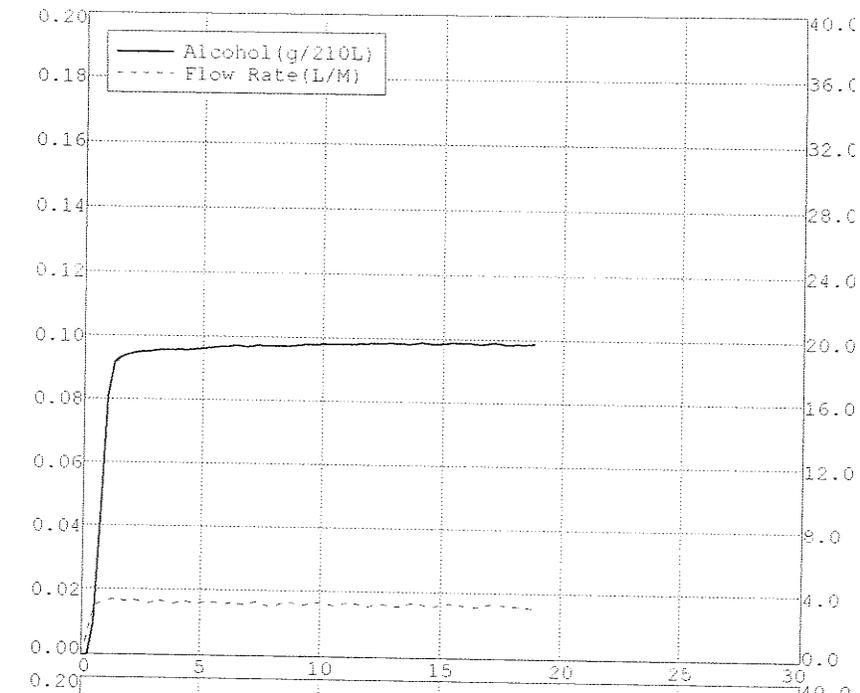

*Charles B. Geisler* #200