

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 02/13/2022

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 21440

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:13
INTERNAL STANDARD	VERIFIED	15:14
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	15:14
BLANK TEST	0.00	15:15
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	15:15
BLANK TEST	0.00	15:16
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	15:16
BLANK TEST	0.00	15:17

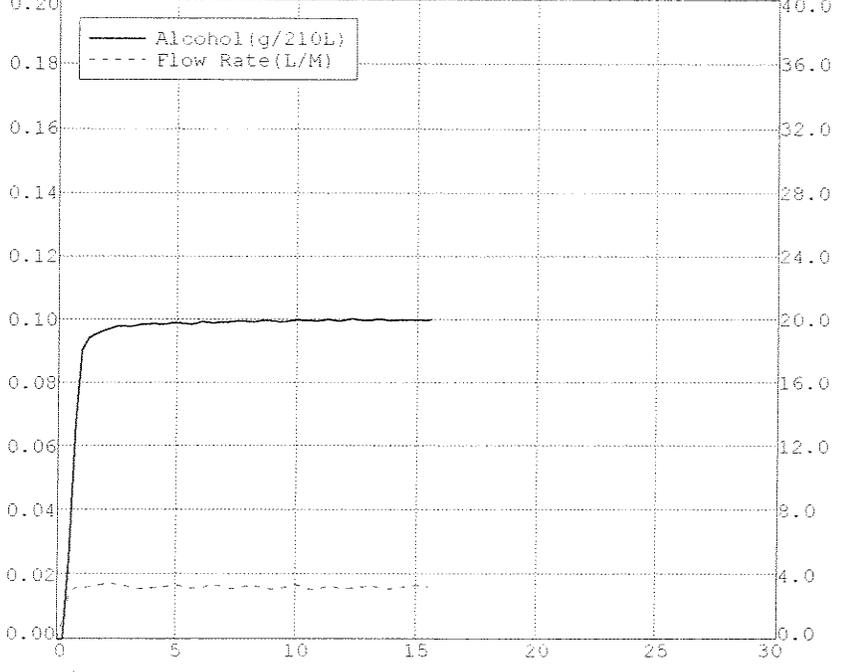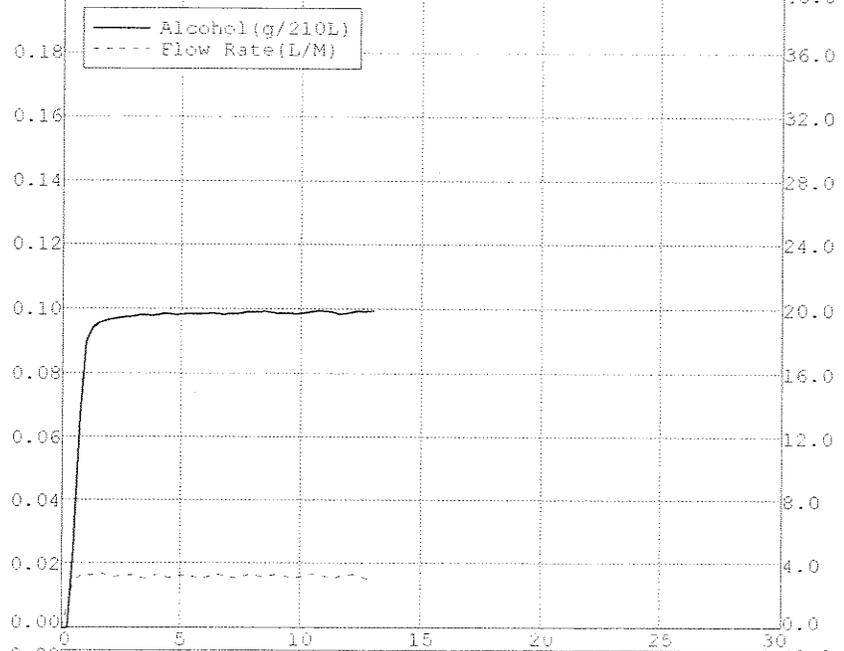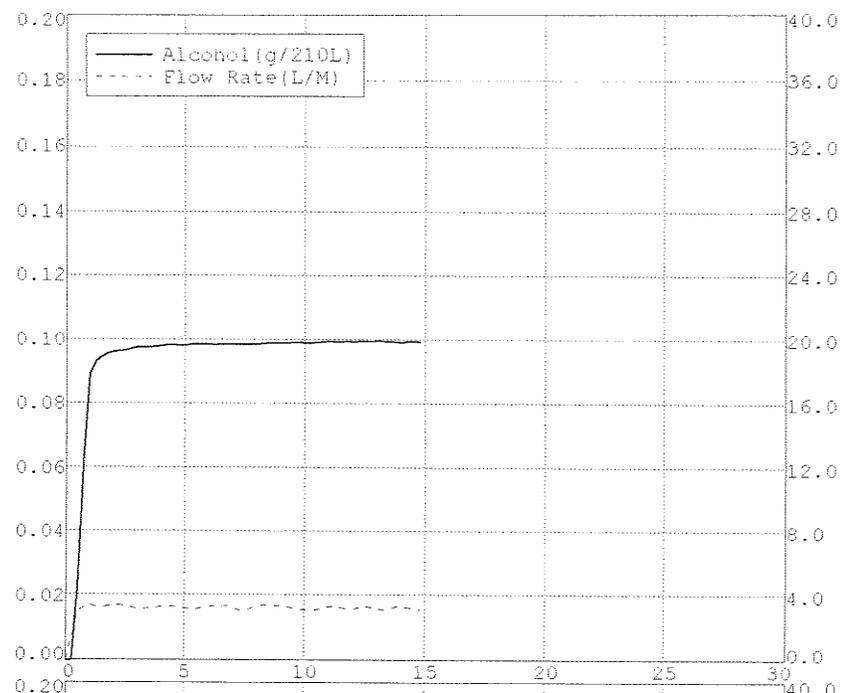

Handwritten signature: C. B. Geisler