

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 04/08/2022

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 22030

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:08
INTERNAL STANDARD	VERIFIED	15:08
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	15:09
BLANK TEST	0.00	15:10
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	15:10
BLANK TEST	0.00	15:11
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	15:11
BLANK TEST	0.00	15:12

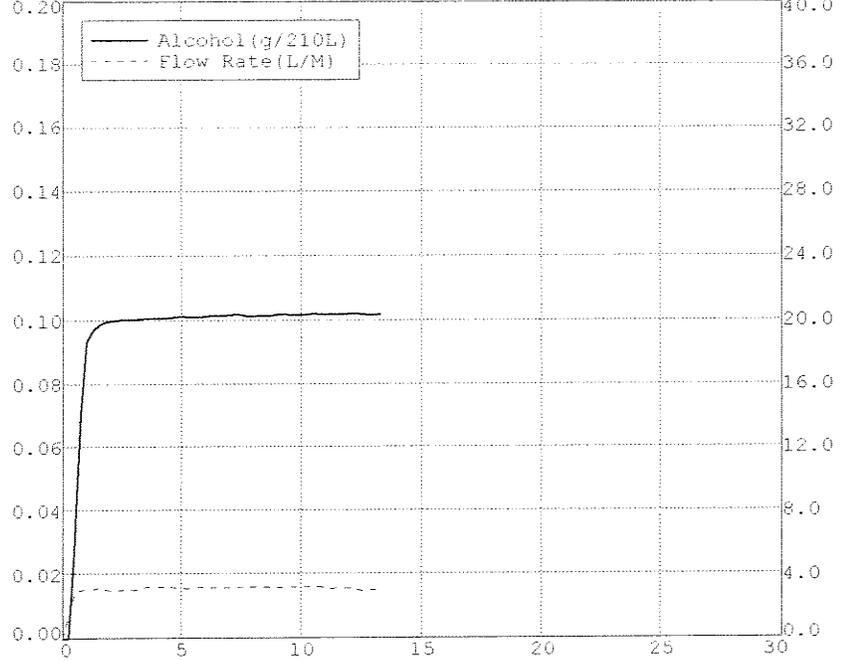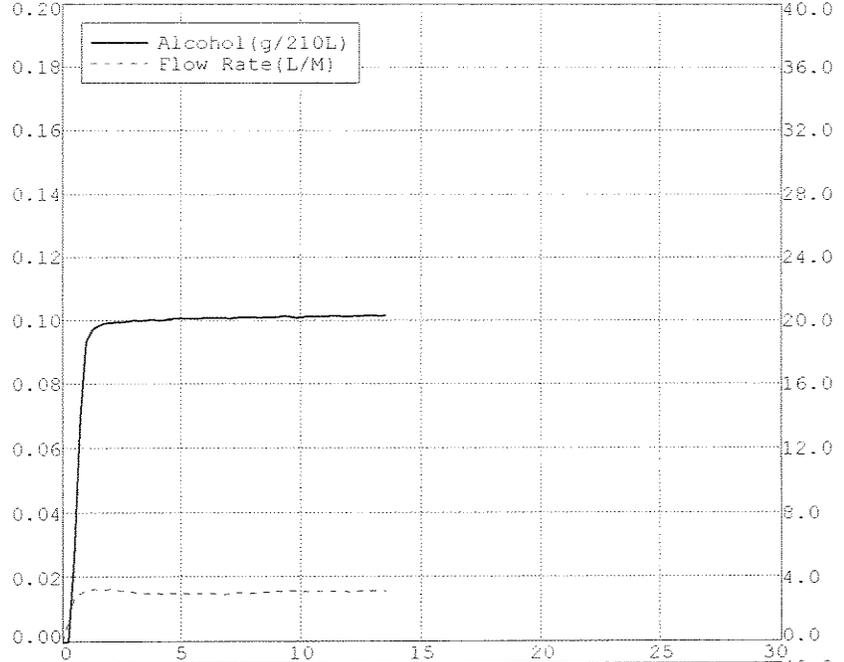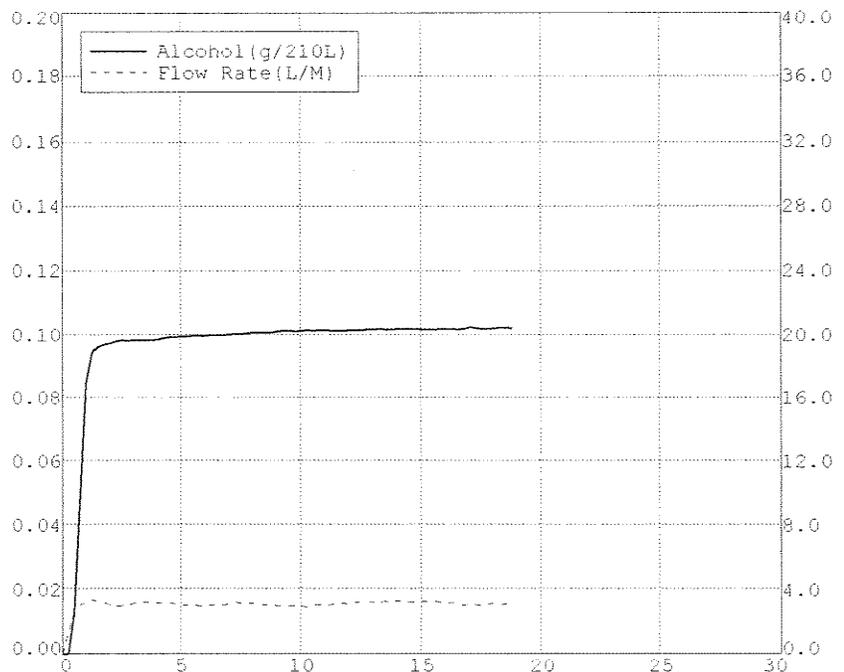

Handwritten signature: C. B. Geisler #247