

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 04/14/2022

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 22030

Nominal = 0.10 g/210L

BLANK TEST	0.00	14:35
INTERNAL STANDARD	VERIFIED	14:35
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	14:35
BLANK TEST	0.00	14:36
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	14:37
BLANK TEST	0.00	14:38
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	14:38
BLANK TEST	0.00	14:39

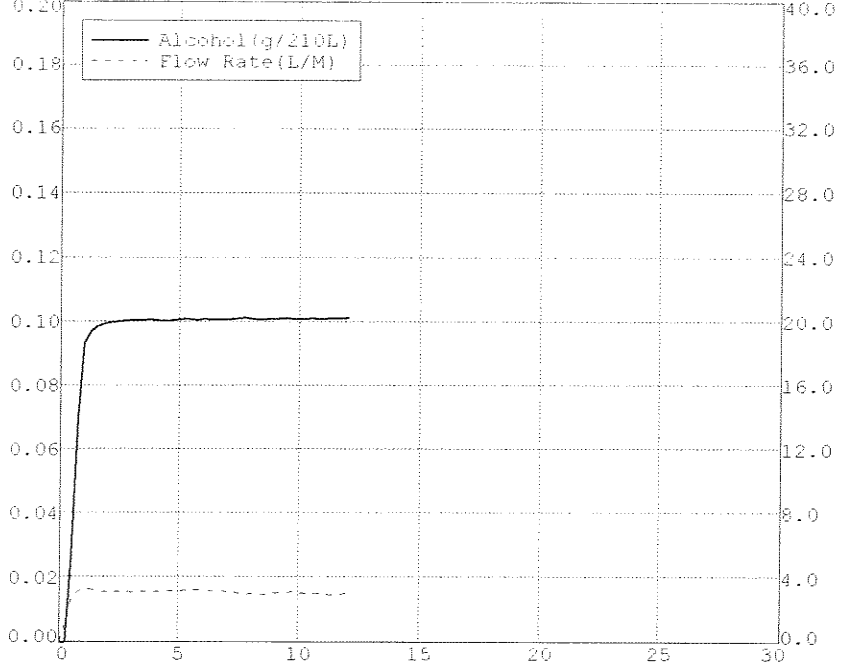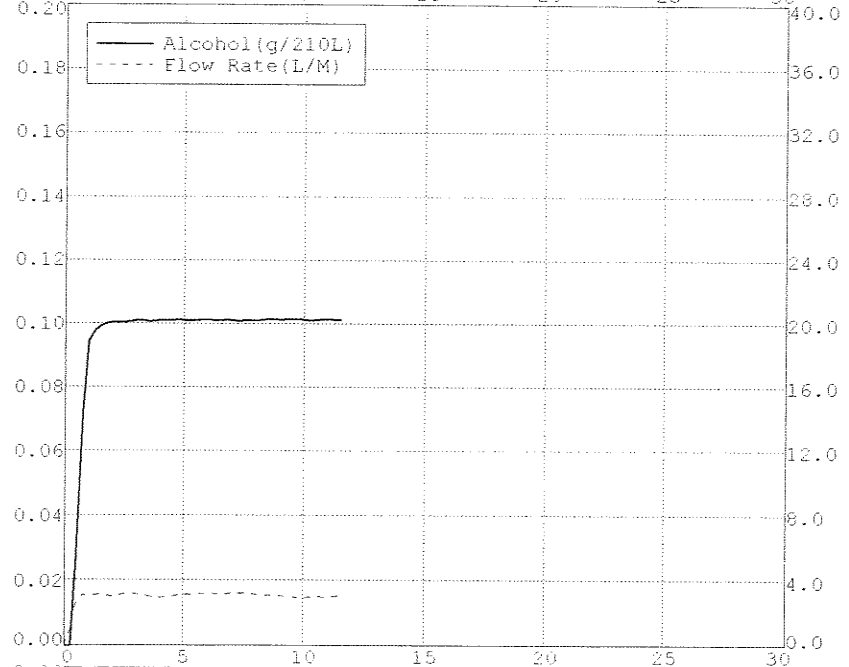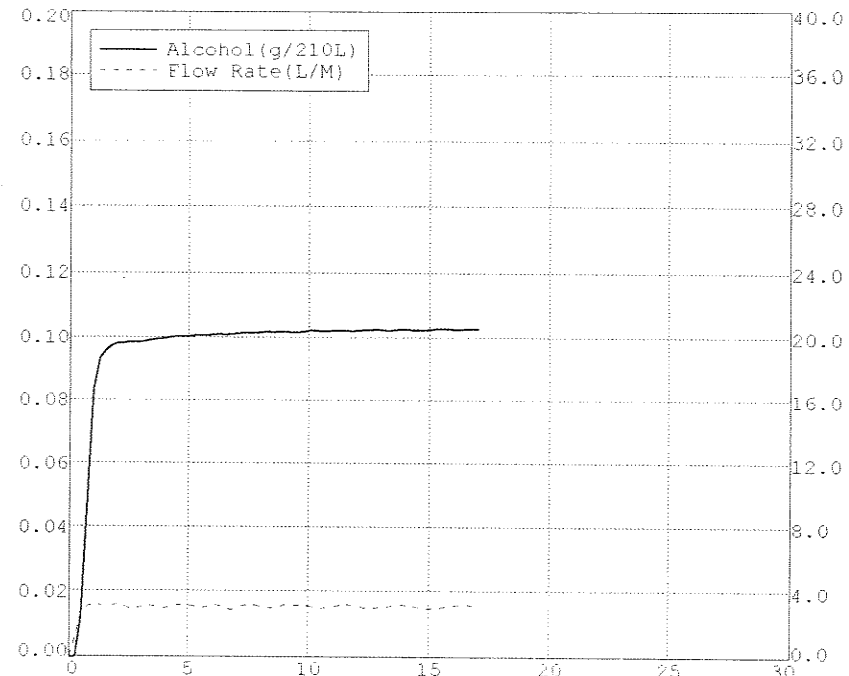

Handwritten signature: J. Charles Geisler #244