

SOLUTION CHANGE




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 05/02/2022

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 22030

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:59
INTERNAL STANDARD	VERIFIED	16:59
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	16:59
BLANK TEST	0.00	17:00
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	17:00
BLANK TEST	0.00	17:01
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	17:02
BLANK TEST	0.00	17:02

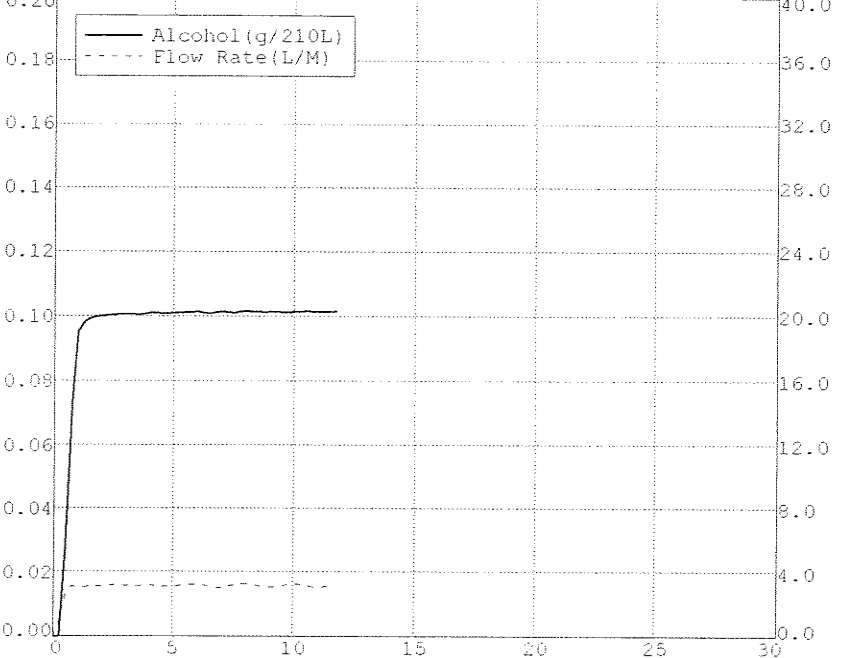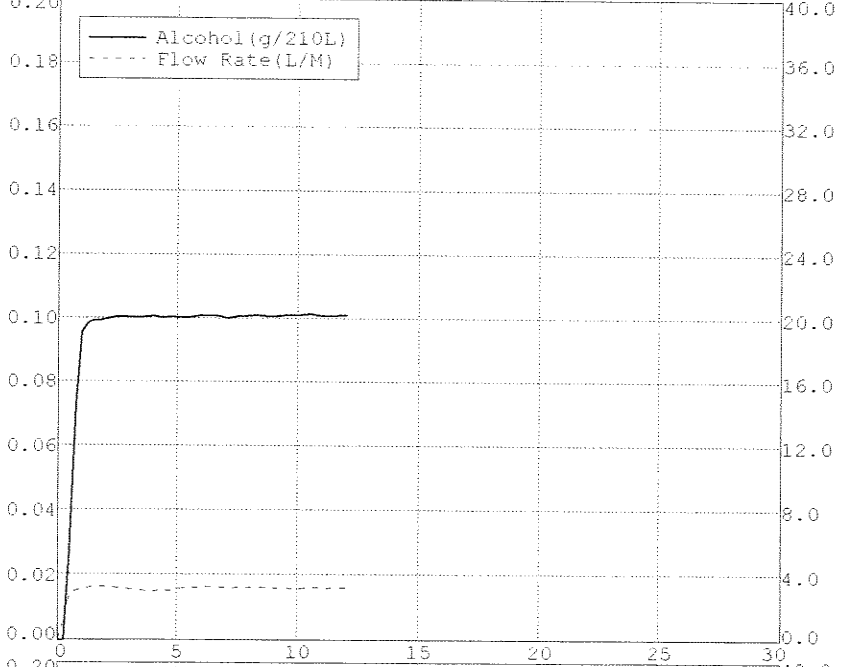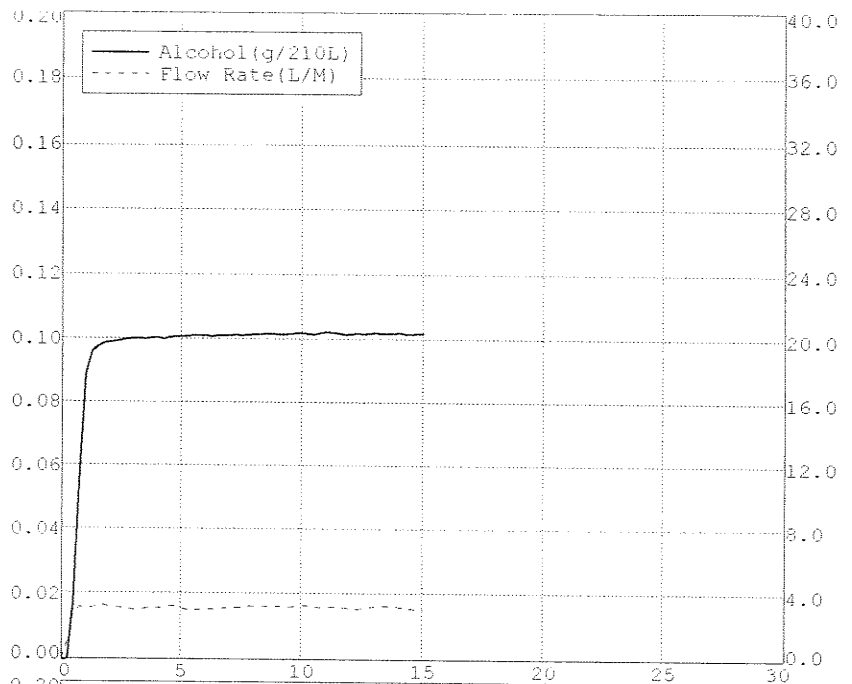

*Chl. B. #241*