

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 06/08/2022

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN COUNTY
SHERIFF'S OFFICE
Reference Standard #: 22100

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:22
INTERNAL STANDARD	VERIFIED	18:22
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:22
BLANK TEST	0.00	18:23
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:24
BLANK TEST	0.00	18:24
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:25
BLANK TEST	0.00	18:26

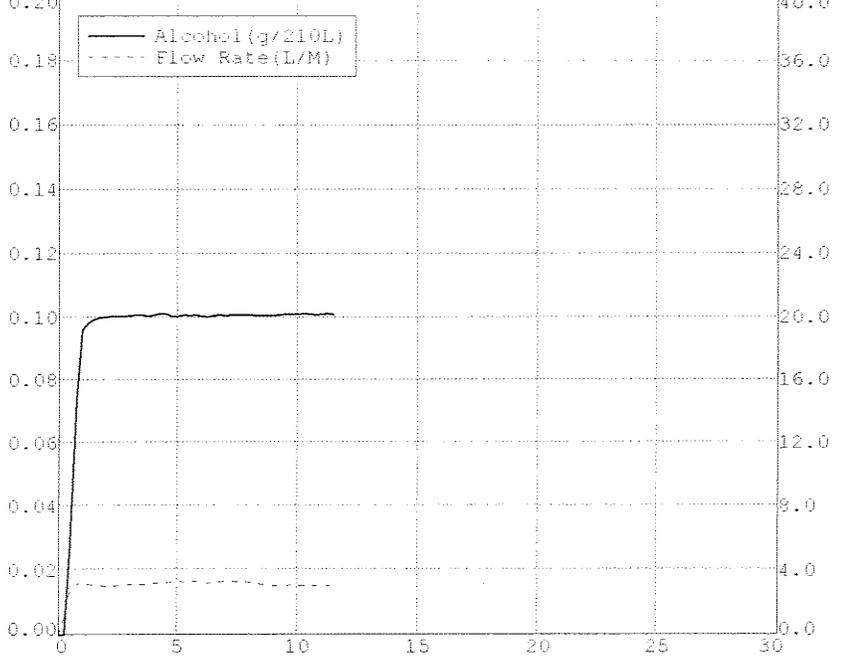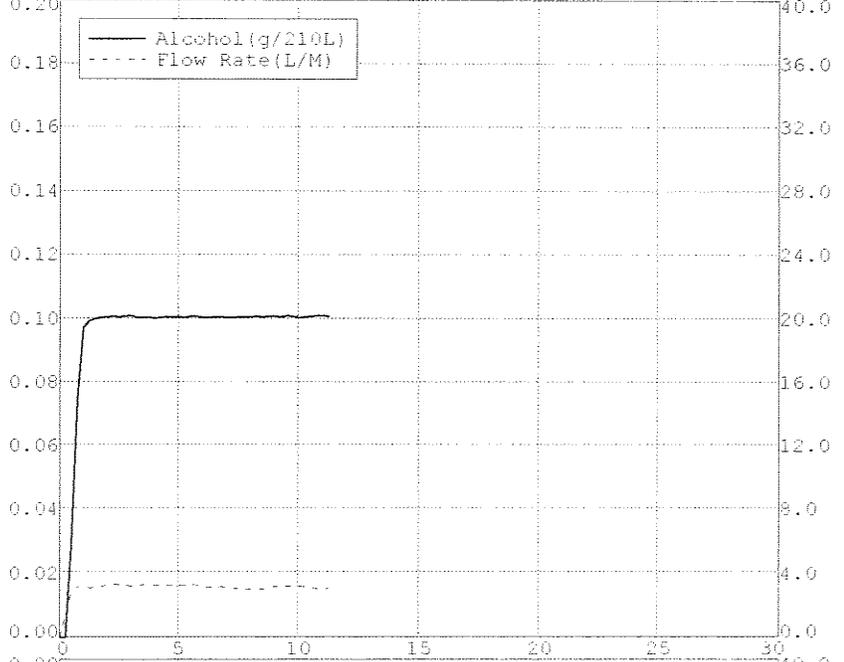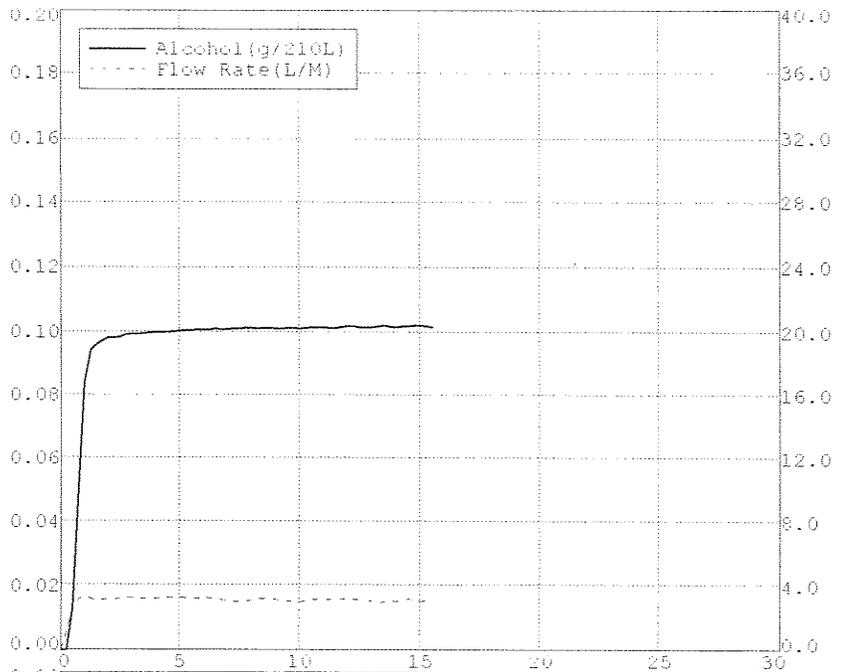

Handwritten signature: C.B. Geisler #221