

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 06/18/2022

OPERATOR NAME:  
MICHAEL A CAMPBELL  
Permit #: 42422  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 22100

Nominal = 0.10 g/210L

BLANK TEST	0.00	06:57
INTERNAL STANDARD	VERIFIED	06:57
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	06:58
BLANK TEST	0.00	06:59
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	06:59
BLANK TEST	0.00	07:00
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	07:00
BLANK TEST	0.00	07:01

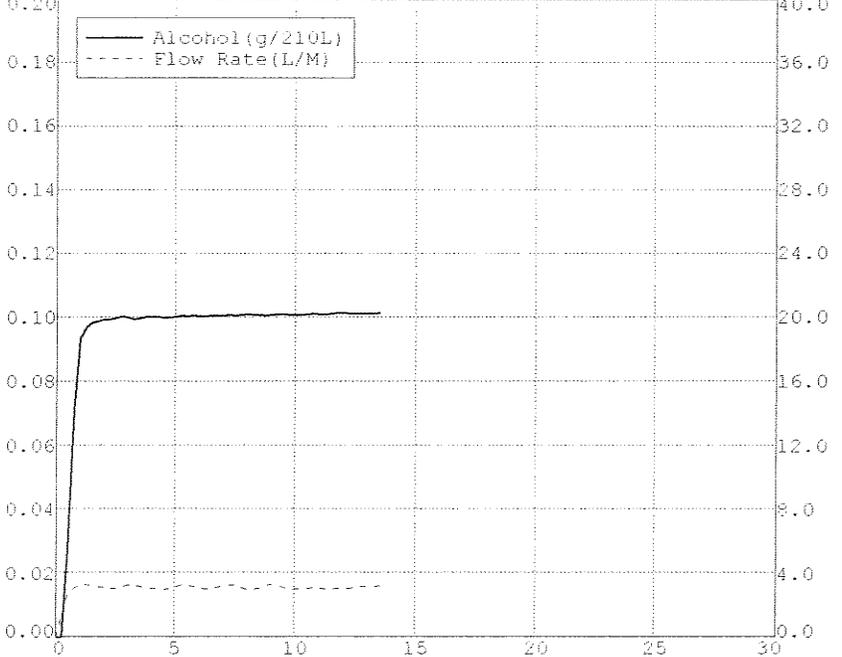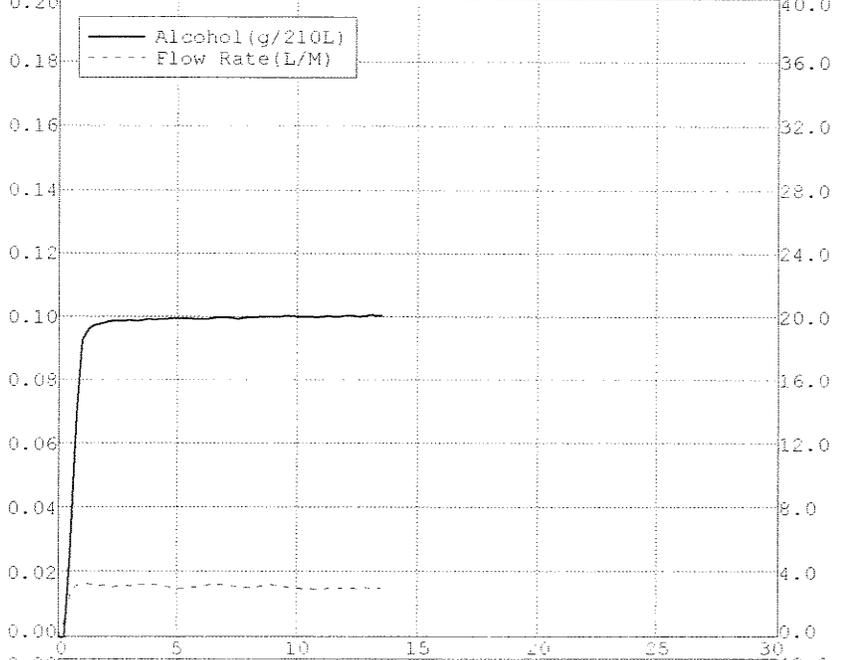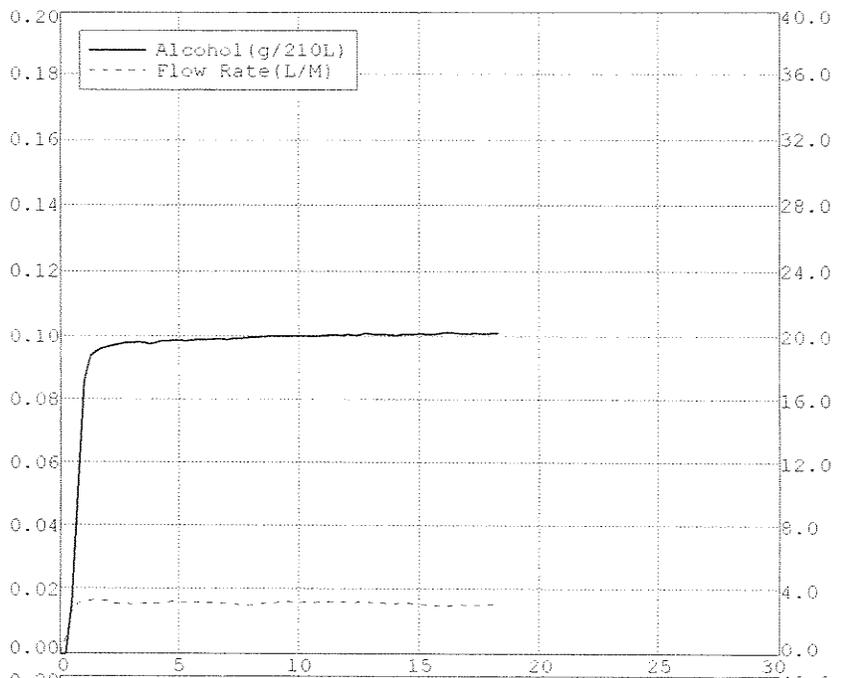

*Michael A Campbell* #757