

SOLUTION CHANGE




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 07/25/2022

OPERATOR NAME:
JOHN D BATEHOLTS
Permit #: 43007
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 22100

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 16:36 |
| INTERNAL STANDARD | VERIFIED | 16:36 |
| REFERENCE STANDARD TEMP | 34.02c | |
| REFERENCE STANDARD | 0.10 | 16:37 |
| BLANK TEST | 0.00 | 16:38 |
| REFERENCE STANDARD TEMP | 34.02c | |
| REFERENCE STANDARD | 0.10 | 16:38 |
| BLANK TEST | 0.00 | 16:39 |
| REFERENCE STANDARD TEMP | 34.02c | |
| REFERENCE STANDARD | 0.10 | 16:39 |
| BLANK TEST | 0.00 | 16:40 |

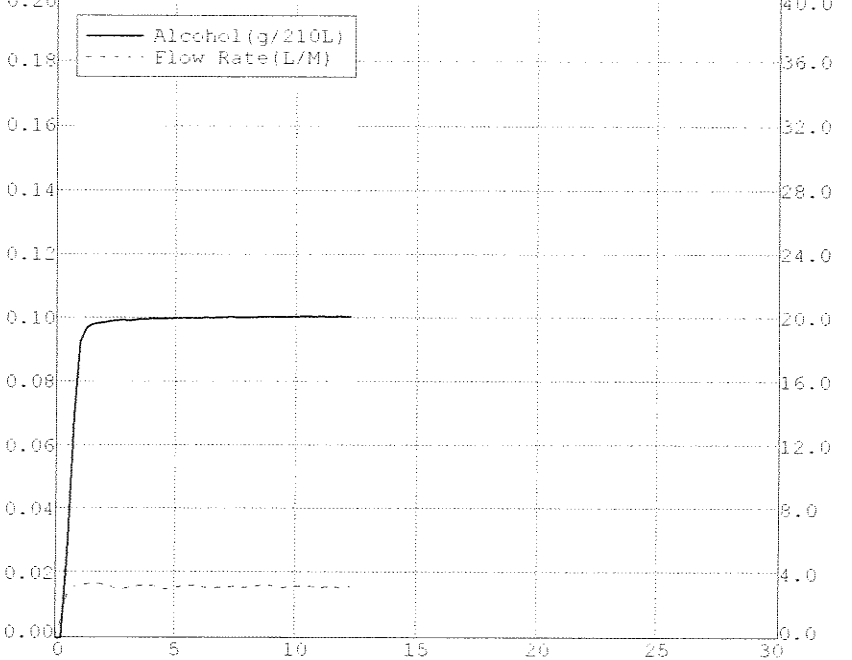

J. D. Bateholts 07/25