

SUPERVISOR TEST


WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 08/15/2022

OPERATOR NAME:
J RIEHL
Permit #: 47503
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 22190

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:50
INTERNAL STANDARD	VERIFIED	07:50
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	07:50
BLANK TEST	0.00	07:51
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	07:51
BLANK TEST	0.00	07:52
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	07:53
BLANK TEST	0.00	07:54

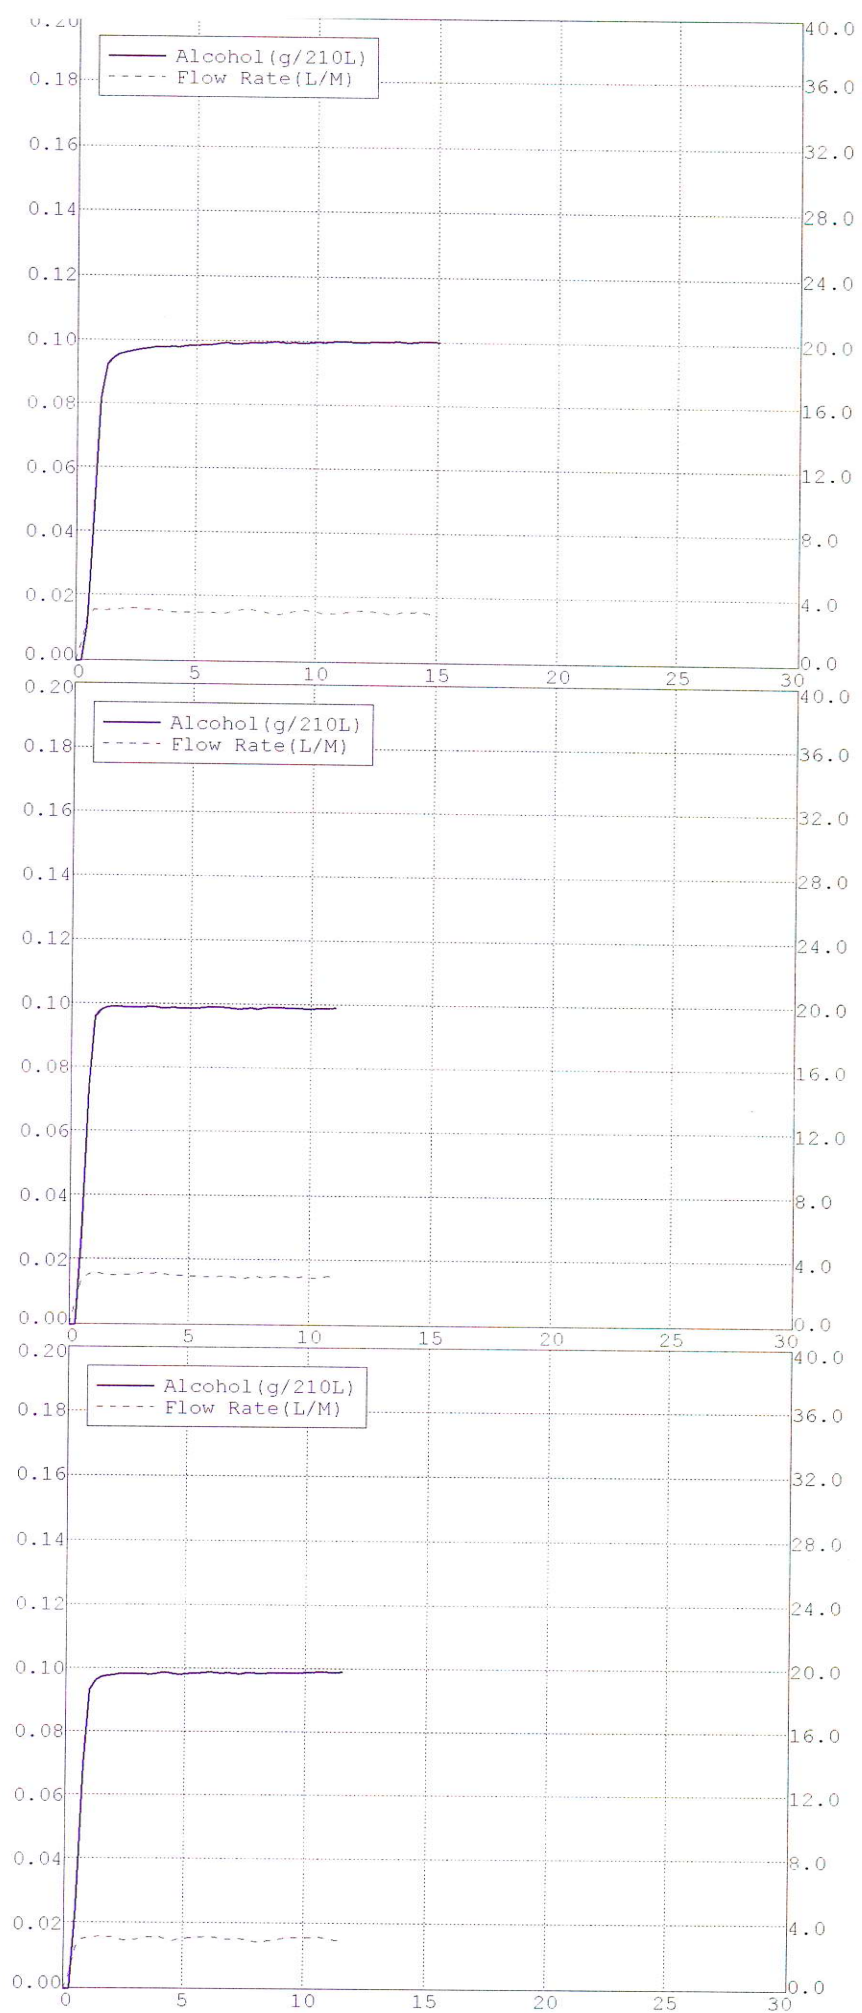

J Riehl
#820