

SOLUTION CHANGE


-----  
 WARREN CO.  
 SHERIFF'S OFFICE  
 DATAMASTER dmt: 106606  
 -----

Date: 09/01/2022

OPERATOR NAME:  
 CHARLES B GEISLER  
 Permit #: 33757  
 Operator Agency/Dept: WARREN CO. SO  
 Reference Standard #: 22190

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:30
INTERNAL STANDARD	VERIFIED	12:30
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	12:31
BLANK TEST	0.00	12:32
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	12:32
BLANK TEST	0.00	12:33
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	12:33
BLANK TEST	0.00	12:34

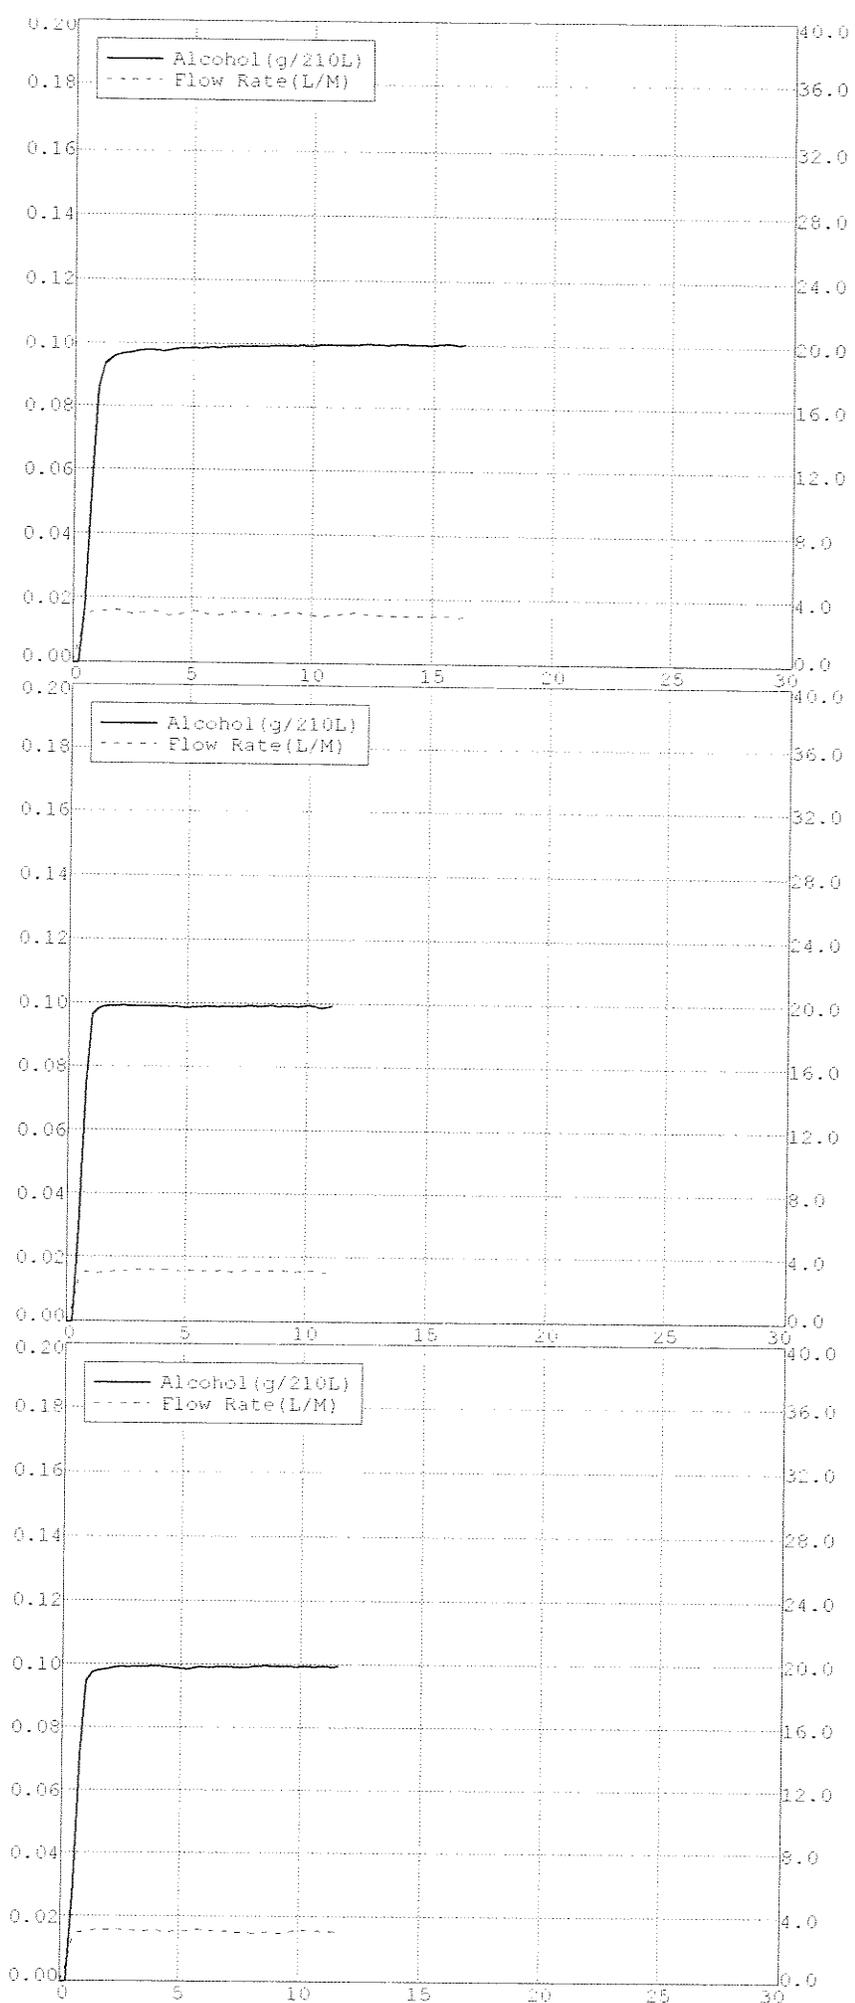

*Sgt. C. B. Geisler #2416*