

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 09/09/2022

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 22190

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:17
INTERNAL STANDARD	VERIFIED	18:17
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:18
BLANK TEST	0.00	18:19
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:19
BLANK TEST	0.00	18:20
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:20
BLANK TEST	0.00	18:21

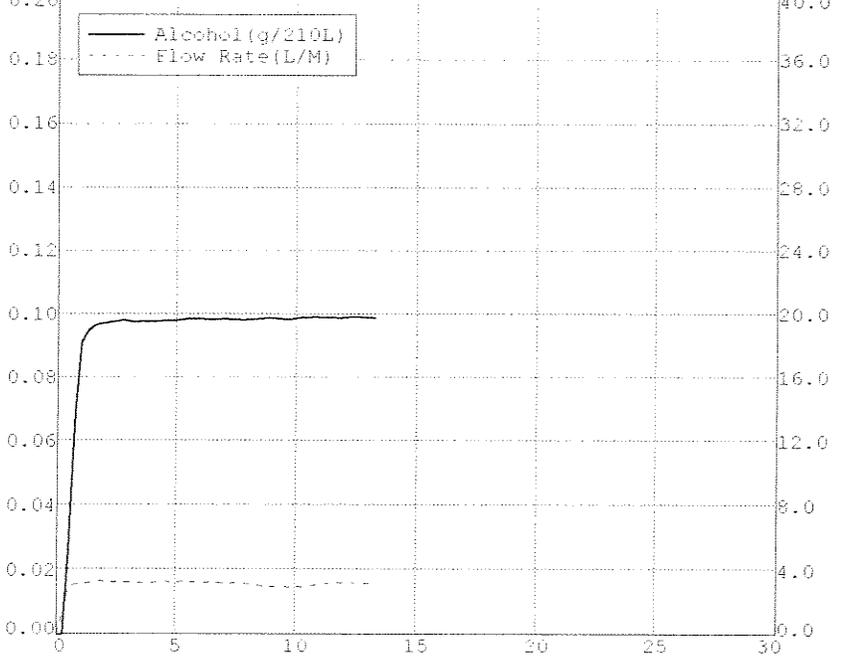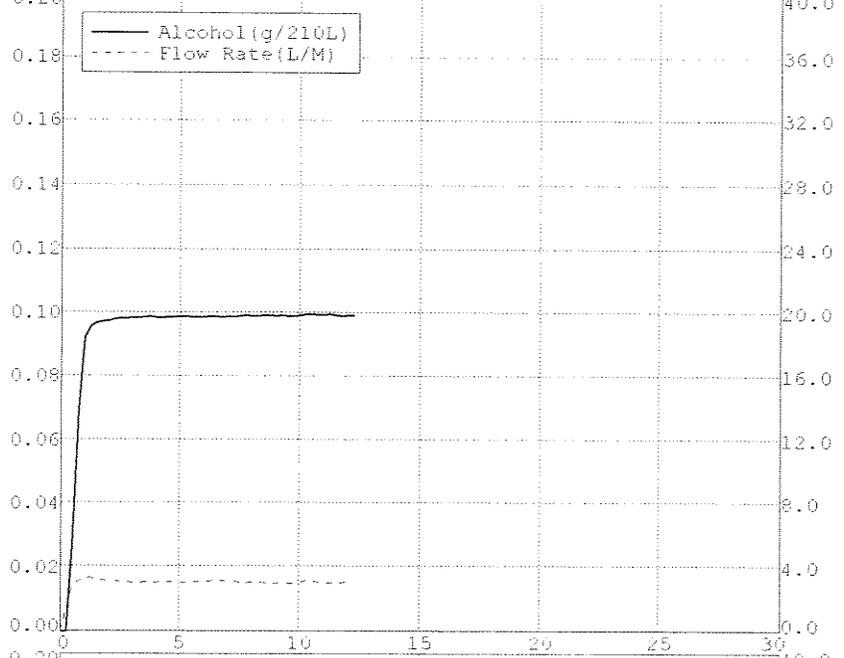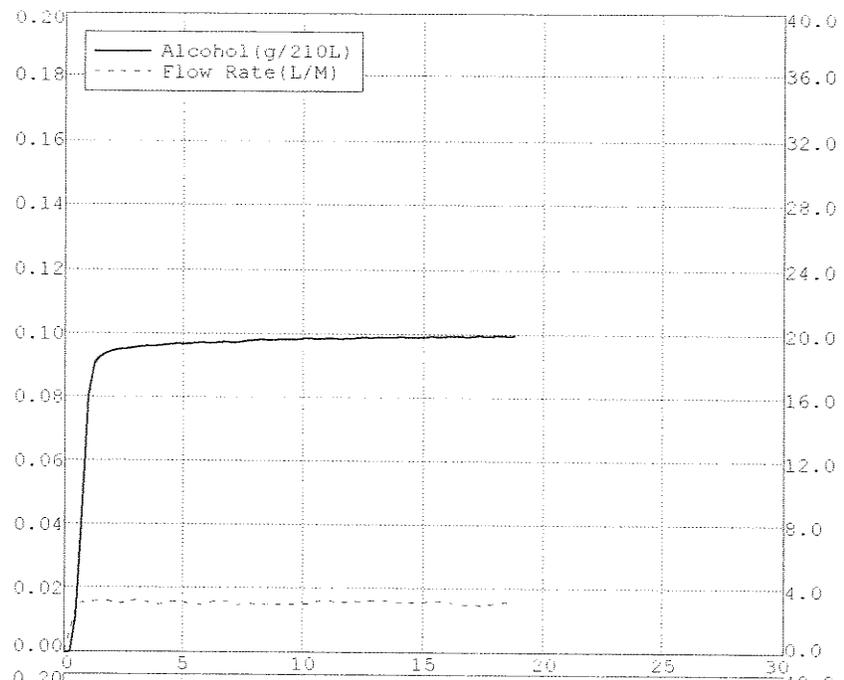

*Sup. Chl-B. All #24v*