

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 09/16/2022

OPERATOR NAME:
MICHAEL A CAMPBELL
Permit #: 42422
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 22190

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:37
INTERNAL STANDARD	VERIFIED	07:38
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	07:38
BLANK TEST	0.00	07:39
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	07:39
BLANK TEST	0.00	07:40
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	07:40
BLANK TEST	0.00	07:41

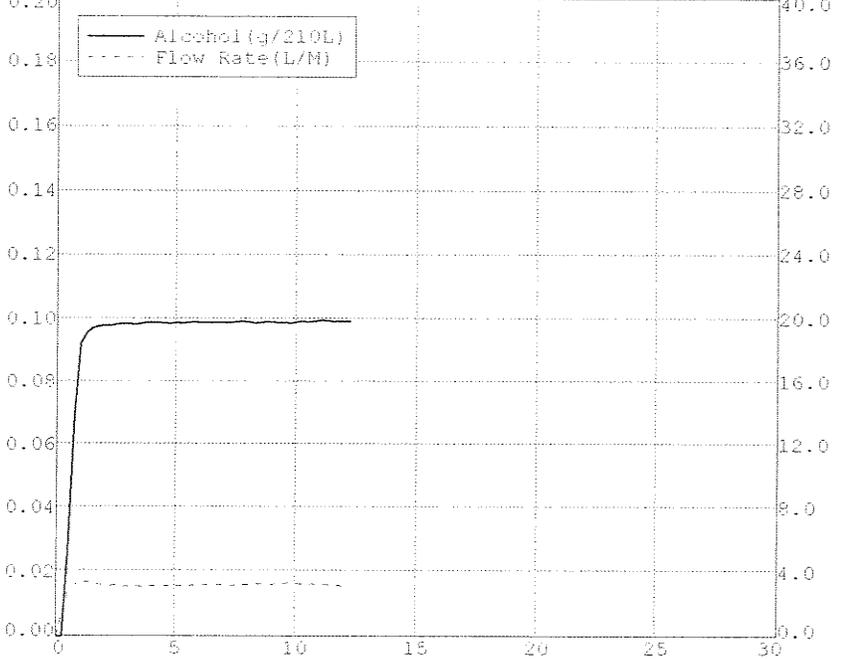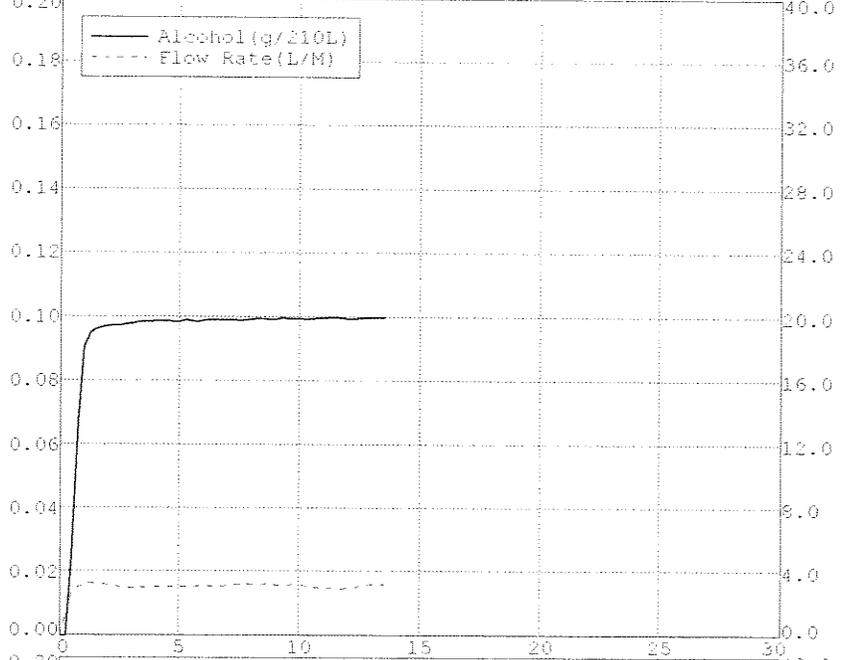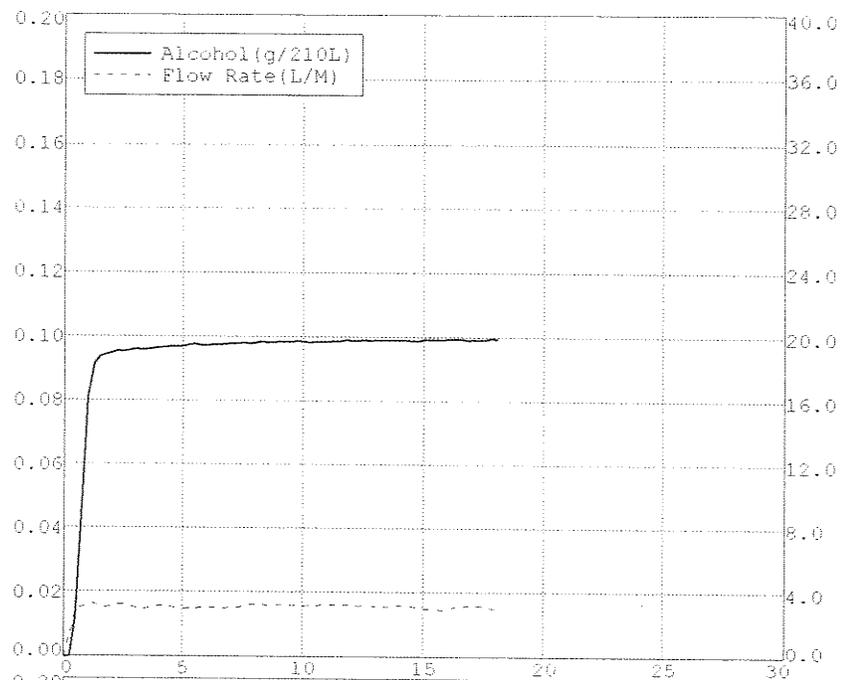

30 *[Signature]* #757