

SOLUTION CHANGE




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 10/03/2022

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 22260

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:22
INTERNAL STANDARD	VERIFIED	13:22
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	13:22
BLANK TEST	0.00	13:23
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	13:24
BLANK TEST	0.00	13:24
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	13:25
BLANK TEST	0.00	13:26

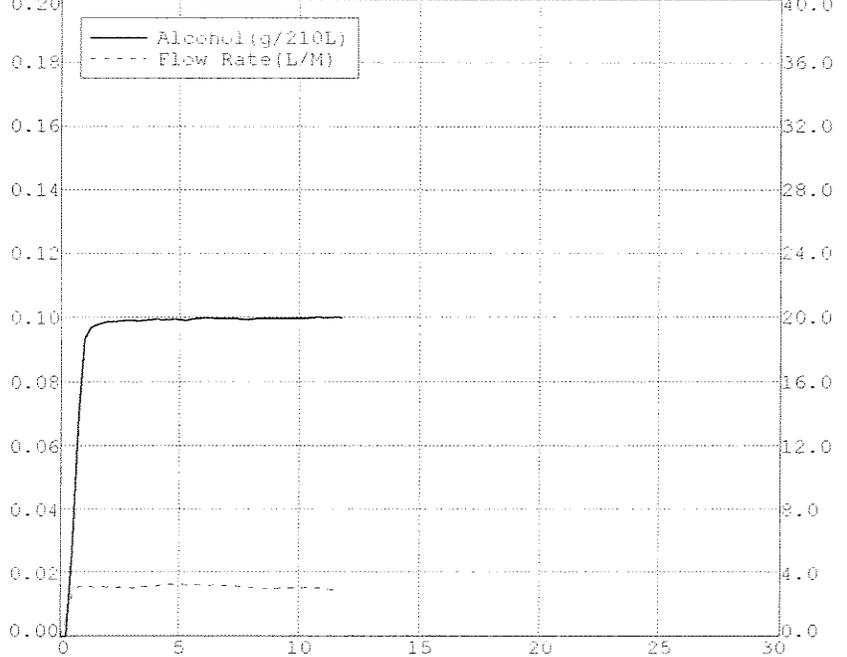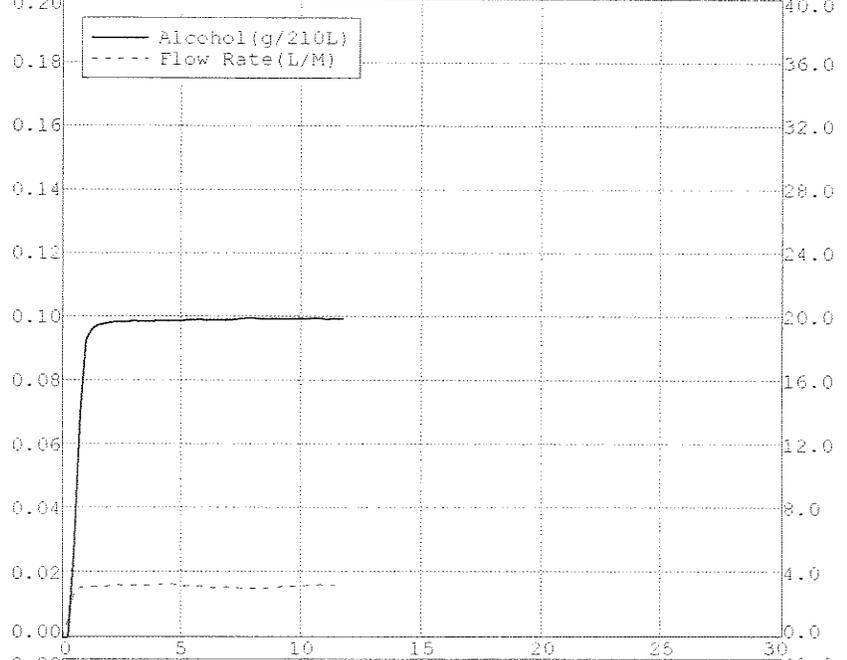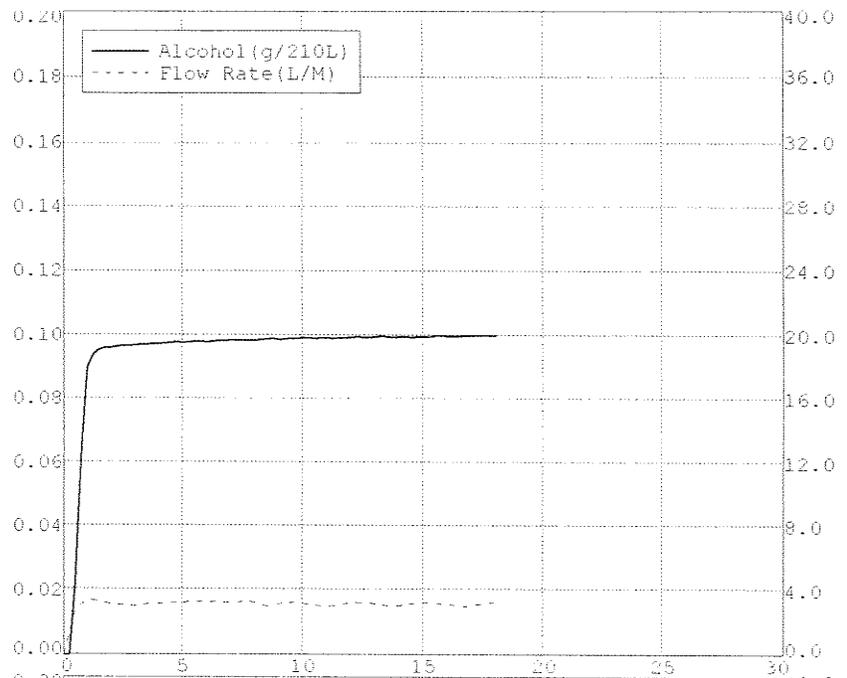

Handwritten signature: J. B. Geisler