

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 10/17/2022

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 22260

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:28
INTERNAL STANDARD	VERIFIED	09:28
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	09:28
BLANK TEST	0.00	09:29
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	09:29
BLANK TEST	0.00	09:30
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	09:31
BLANK TEST	0.00	09:31

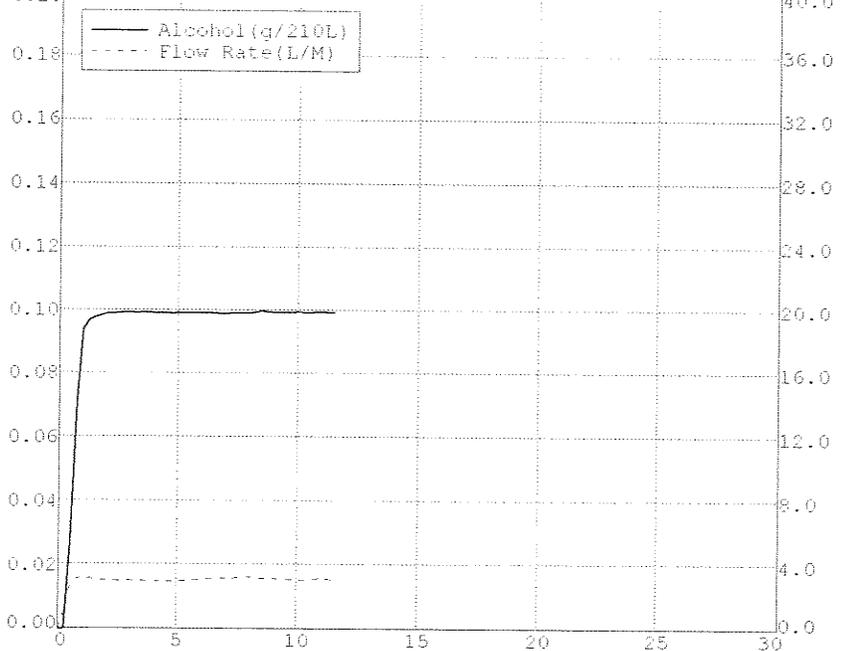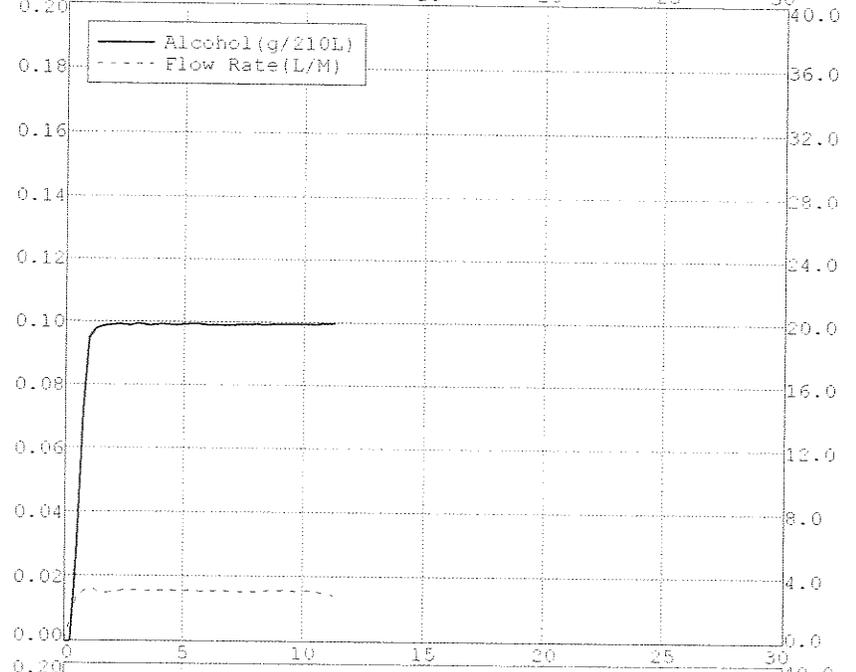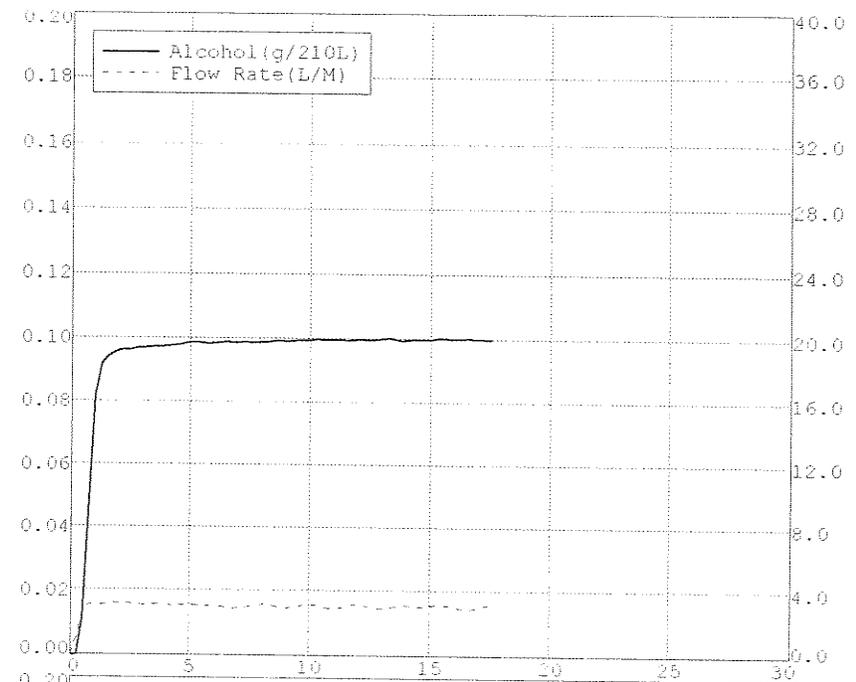

Sgt. Charles B. Geisler #241