

SOLUTION CHANGE




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 11/01/2022

OPERATOR NAME:
JOHN D BATEHOLTS
Permit #: 43007
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 22260

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:22
INTERNAL STANDARD	VERIFIED	08:22
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	08:23
BLANK TEST	0.00	08:24
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	08:24
BLANK TEST	0.00	08:25
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	08:25
BLANK TEST	0.00	08:26

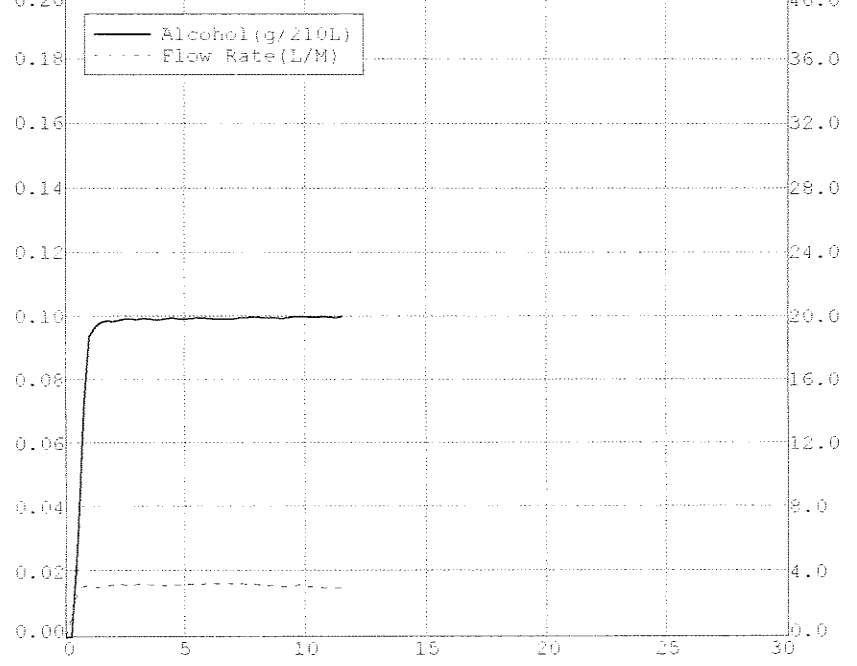

Per *SO* 4714