

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 11/07/2022

OPERATOR NAME:  
MICHAEL A CAMPBELL  
Permit #: 42422  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 22260

Nominal = 0.10 g/210L

BLANK TEST	0.00	06:52
INTERNAL STANDARD	VERIFIED	06:52
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	06:53
BLANK TEST	0.00	06:53
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	06:54
BLANK TEST	0.00	06:55
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	06:55
BLANK TEST	0.00	06:56

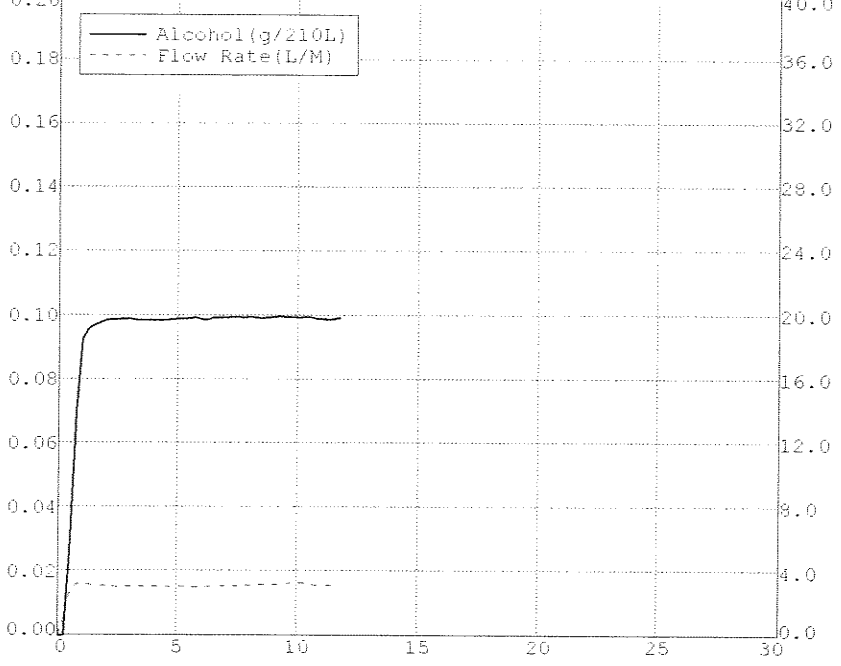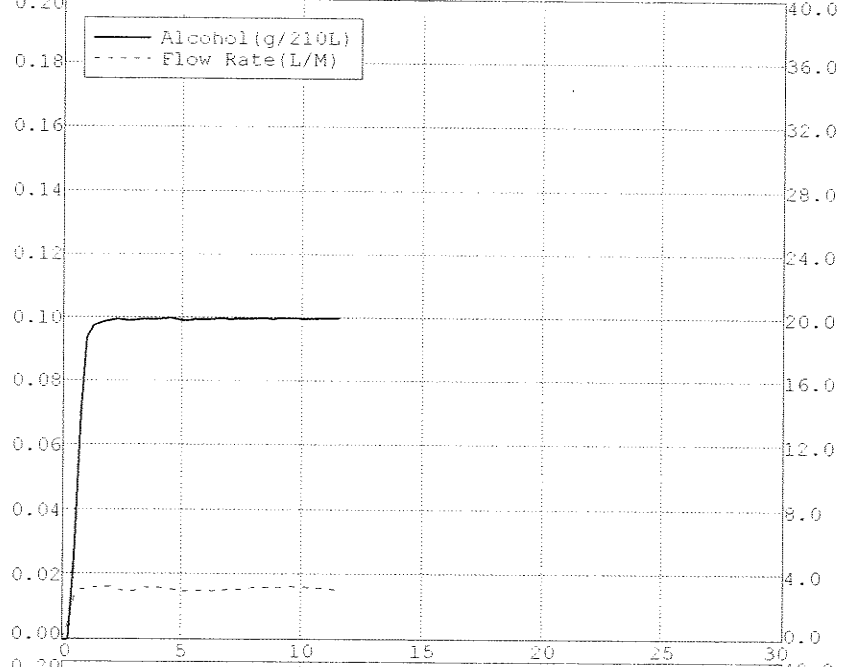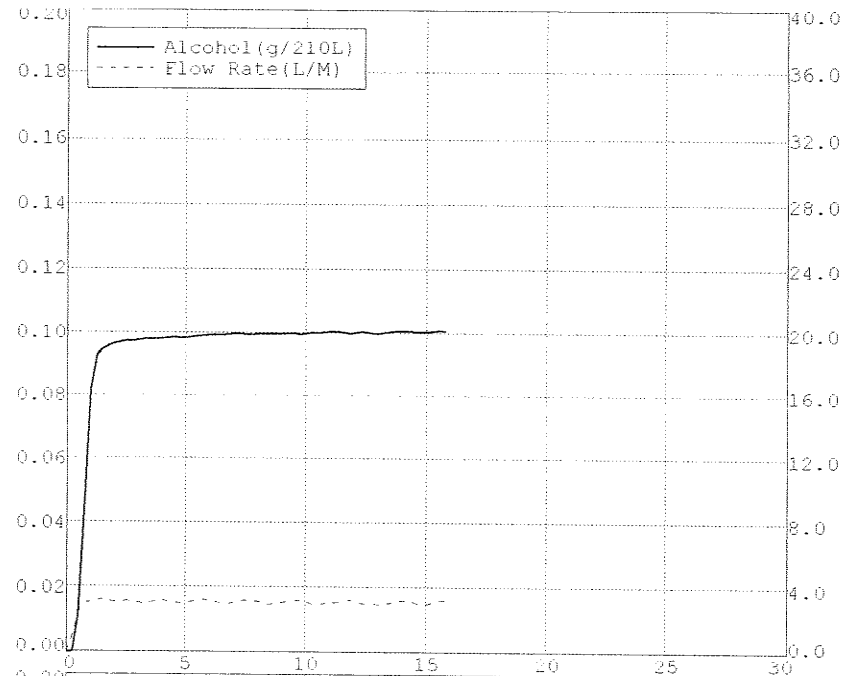

*PO Michael A Campbell 4757*