

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 11/21/2022

OPERATOR NAME:
MICHAEL A CAMPBELL
Permit #: 42422
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 22260

Nominal = 0.10 g/210L

BLANK TEST	0.00	06:57
INTERNAL STANDARD	VERIFIED	06:58
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	06:58
BLANK TEST	0.00	06:59
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	06:59
BLANK TEST	0.00	07:00
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	07:00
BLANK TEST	0.00	07:01

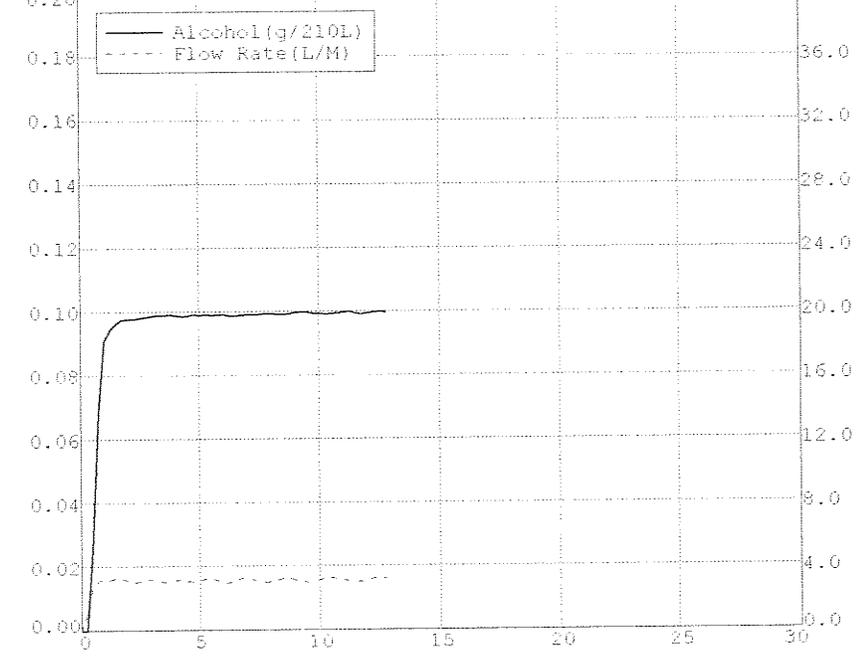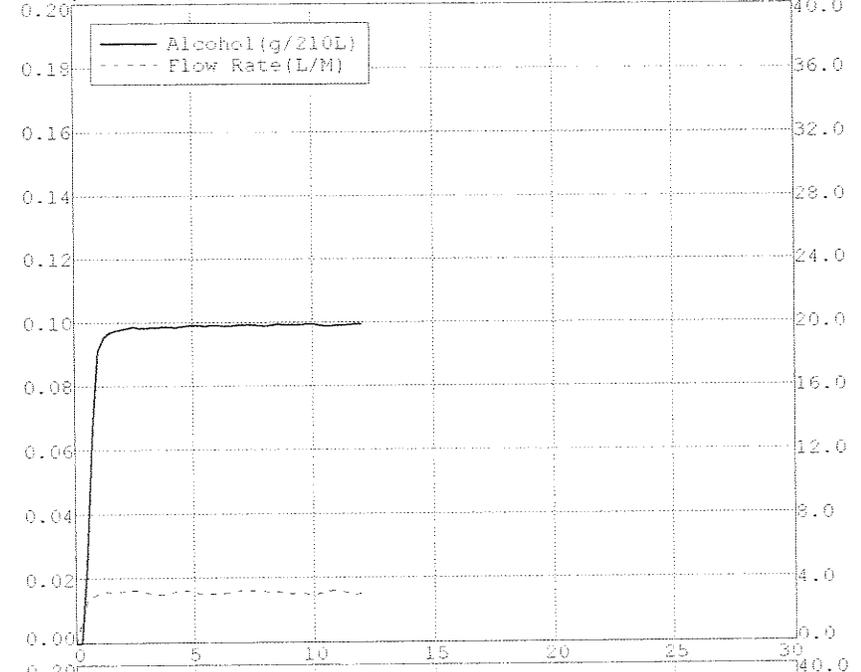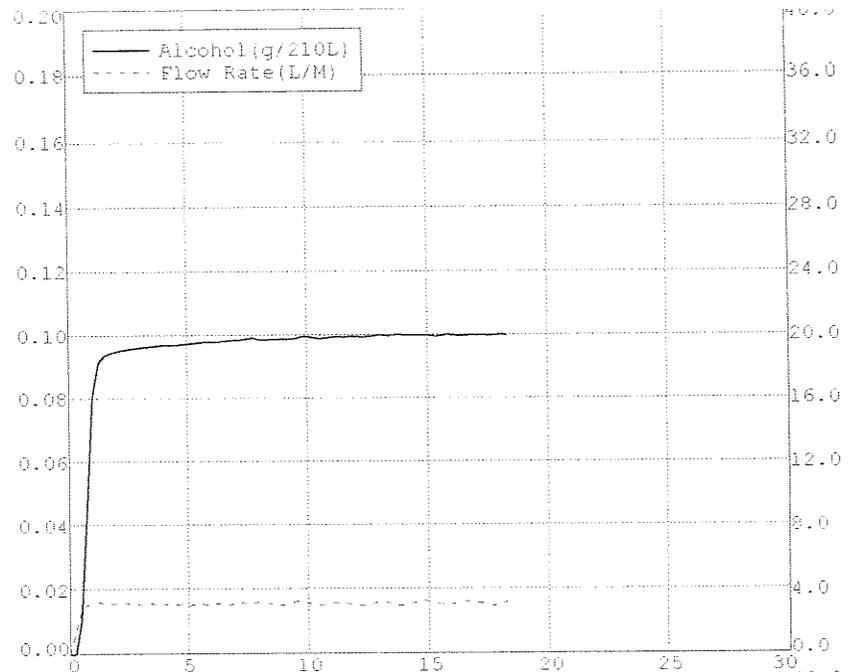

Michael A Campbell #757