

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 12/07/2022

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 22390

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:01
INTERNAL STANDARD	VERIFIED	15:01
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	15:01
BLANK TEST	0.00	15:02
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	15:02
BLANK TEST	0.00	15:03
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	15:03
BLANK TEST	0.00	15:04

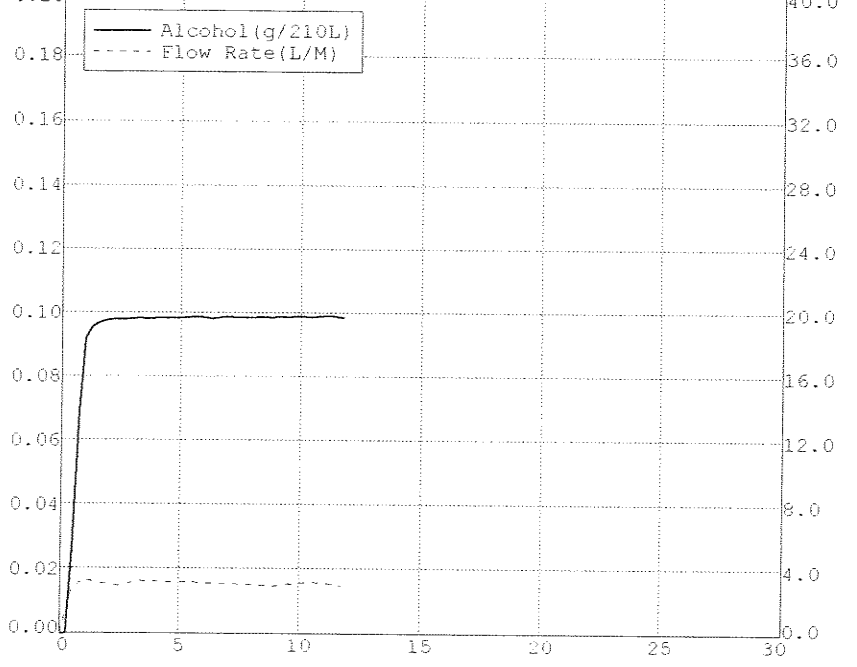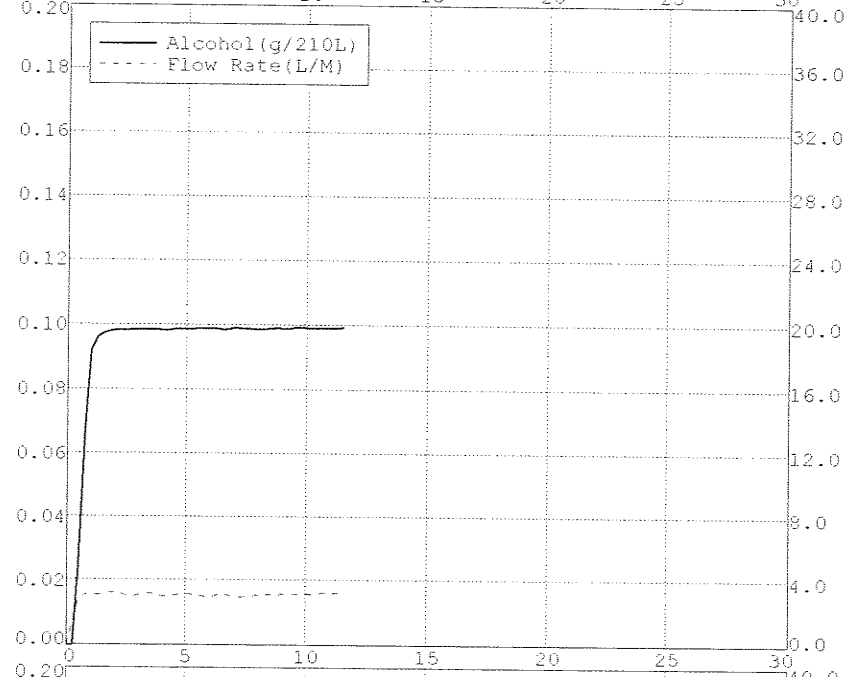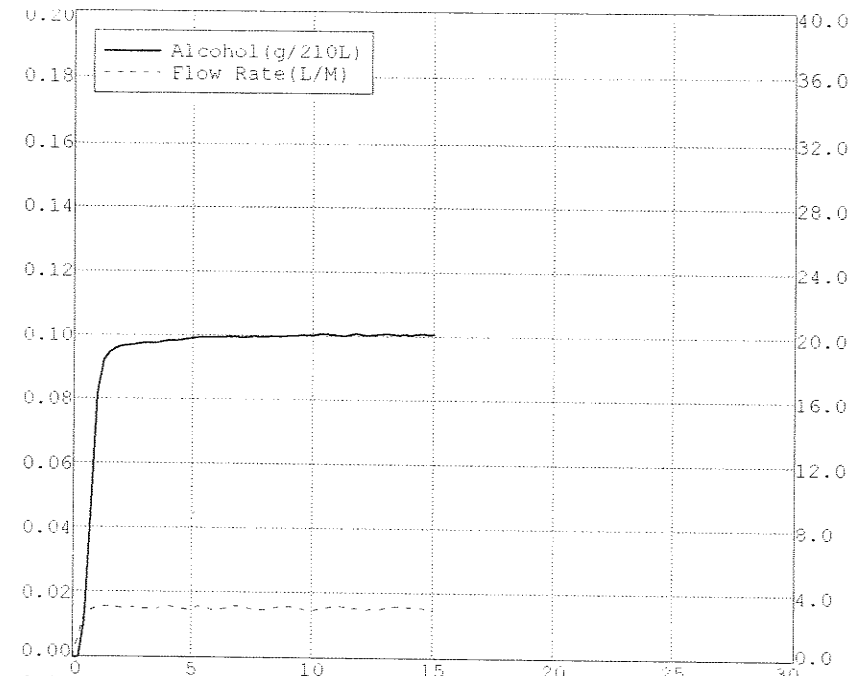

Charles B Geisler #22390