

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 12/19/2022

OPERATOR NAME:
MICHAEL A CAMPBELL
Permit #: 42422
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 22390

Nominal = 0.10 g/210L

BLANK TEST	0.00	06:22
INTERNAL STANDARD	VERIFIED	06:22
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	06:23
BLANK TEST	0.00	06:24
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	06:24
BLANK TEST	0.00	06:25
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	06:25
BLANK TEST	0.00	06:26

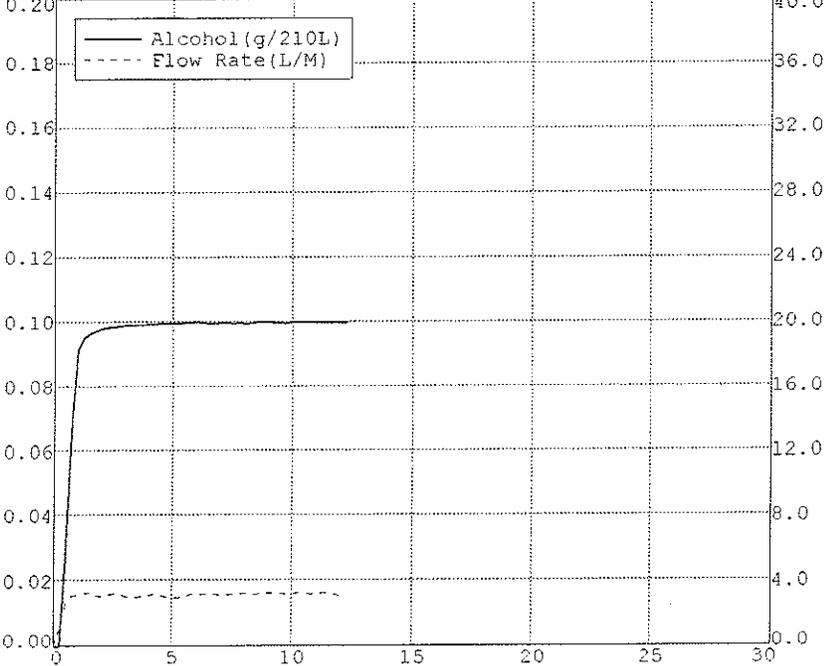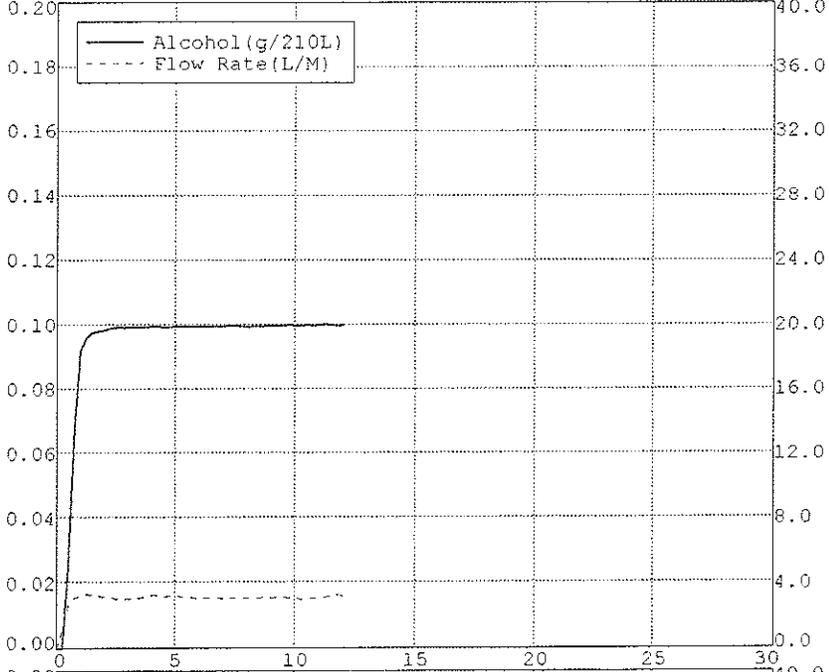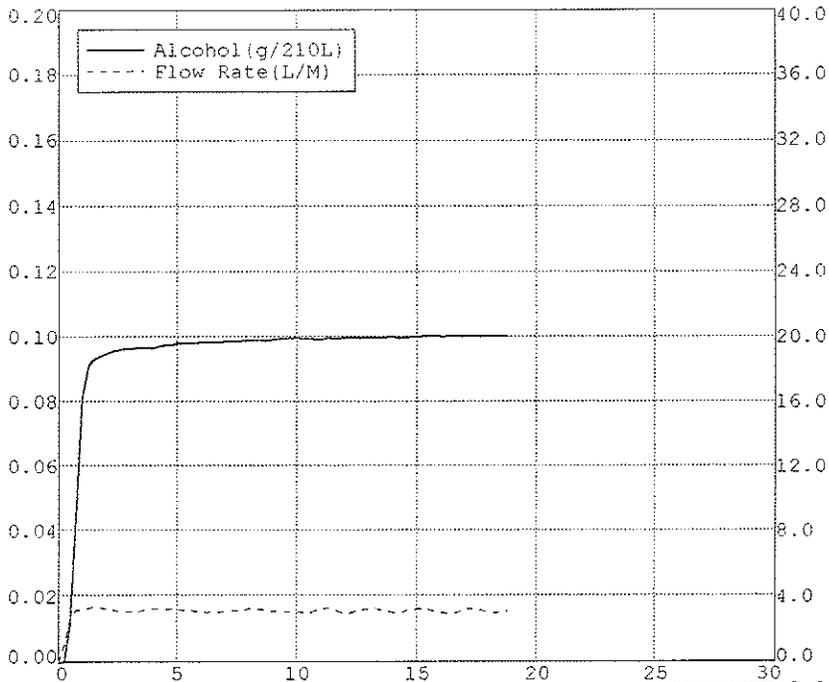

Michael A Campbell #157