

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 12/26/2022

OPERATOR NAME:
SEAN T SMITH
Permit #: 46227
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 22390

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:17
INTERNAL STANDARD	VERIFIED	08:17
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	08:17
BLANK TEST	0.00	08:18
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	08:18
BLANK TEST	0.00	08:19
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	08:20
BLANK TEST	0.00	08:20

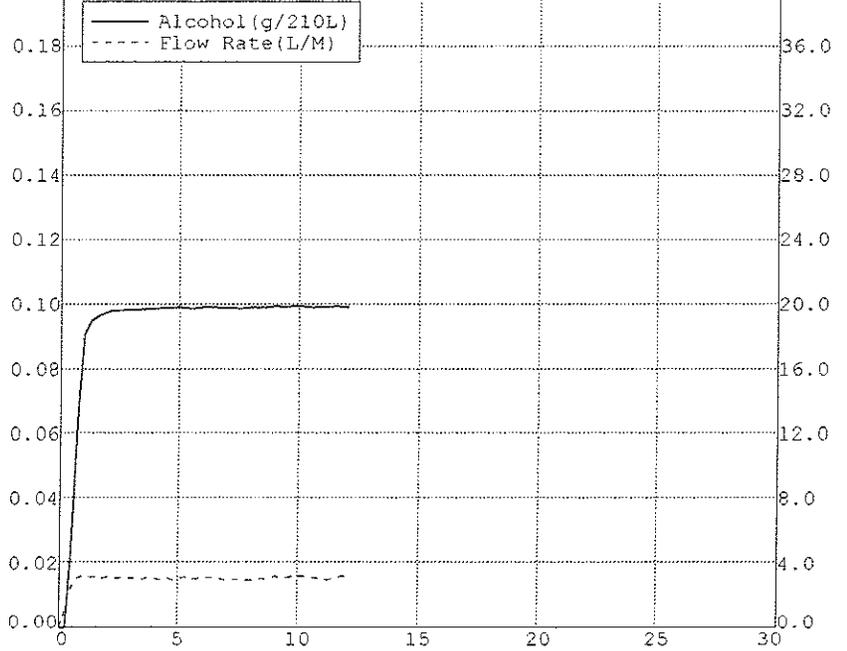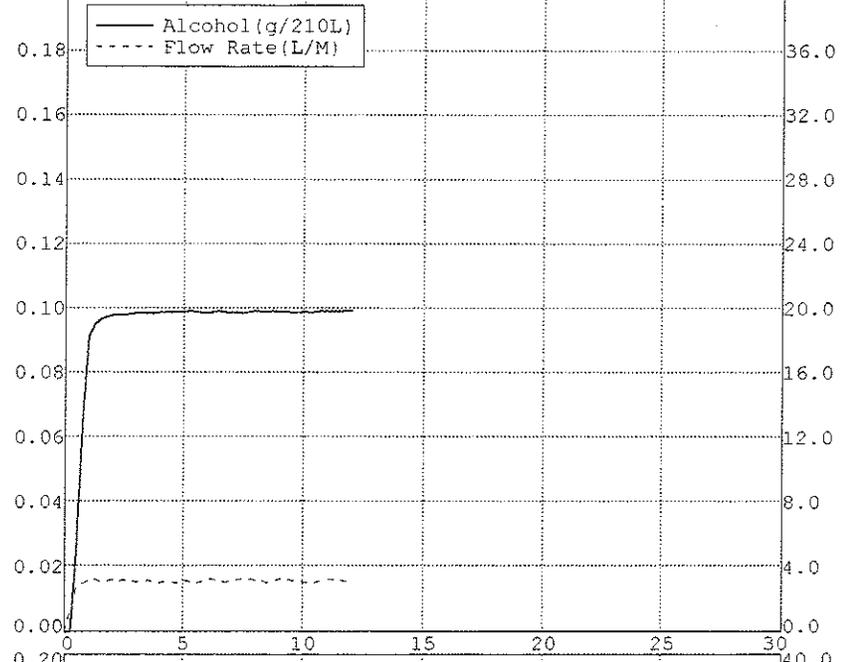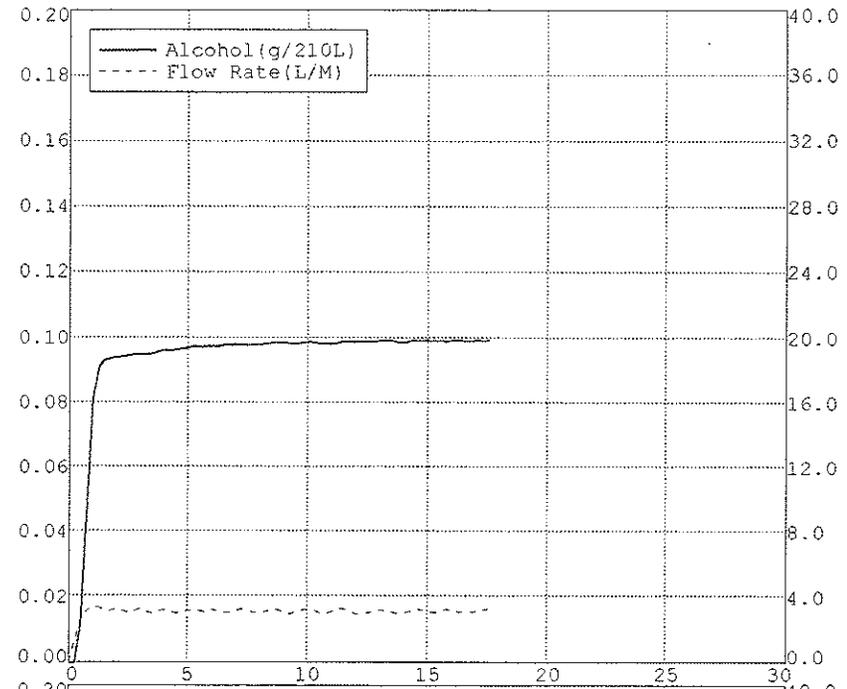

Signature 8/15