

SOLUTION CHANGE




WARREN COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 01/01/2022

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 21390

Nominal = 0.10 g/210L

BLANK TEST	0.00	14:02
INTERNAL STANDARD	VERIFIED	14:02
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	14:02
BLANK TEST	0.00	14:03
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	14:03
BLANK TEST	0.00	14:04
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	14:05
BLANK TEST	0.00	14:06

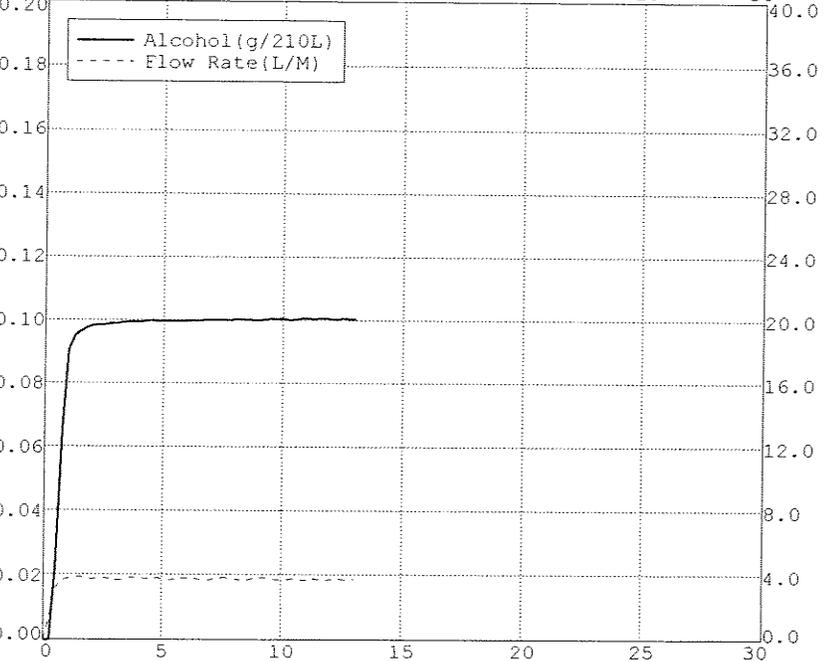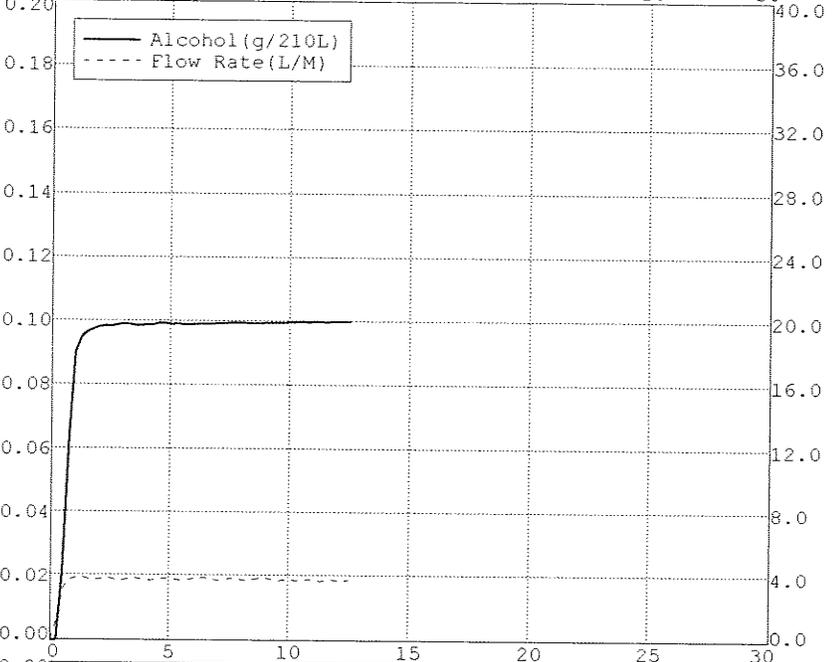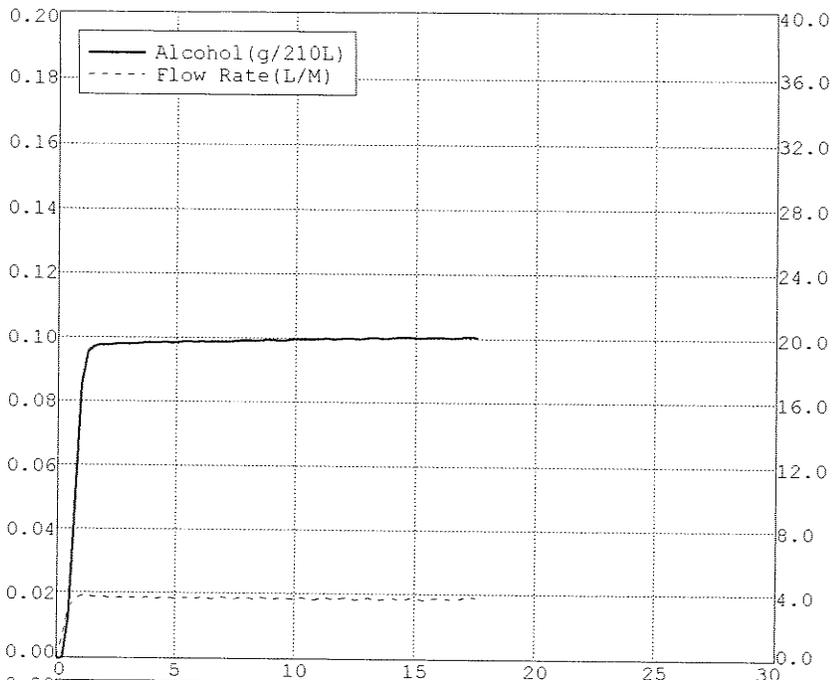

Handwritten signature and initials #2w