

SUPERVISOR TEST




WARREN COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 01/16/2022

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 21390

Nominal = 0.10 g/210L

BLANK TEST	0.00	14:32
INTERNAL STANDARD	VERIFIED	14:32
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	14:32
BLANK TEST	0.00	14:33
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	14:34
BLANK TEST	0.00	14:35
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	14:35
BLANK TEST	0.00	14:36

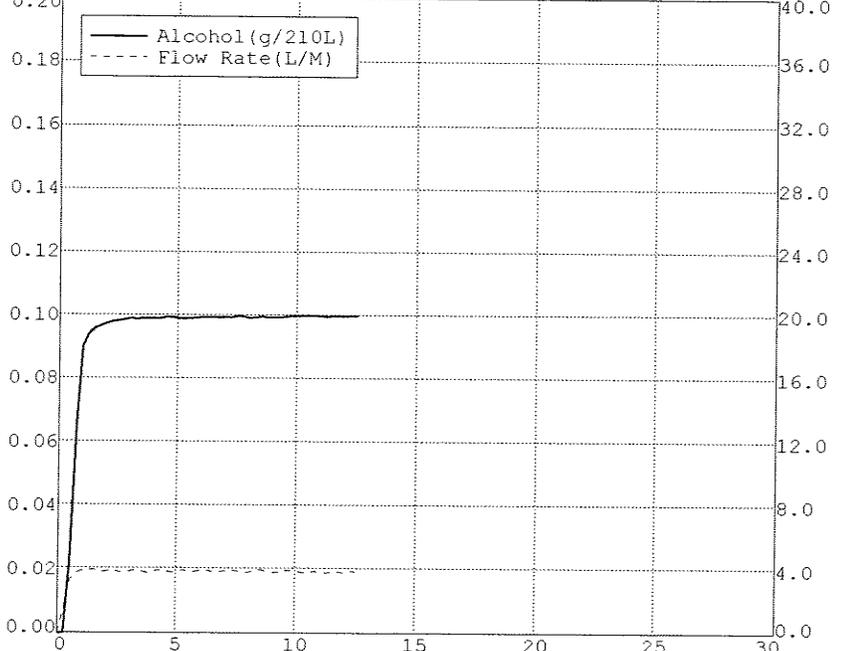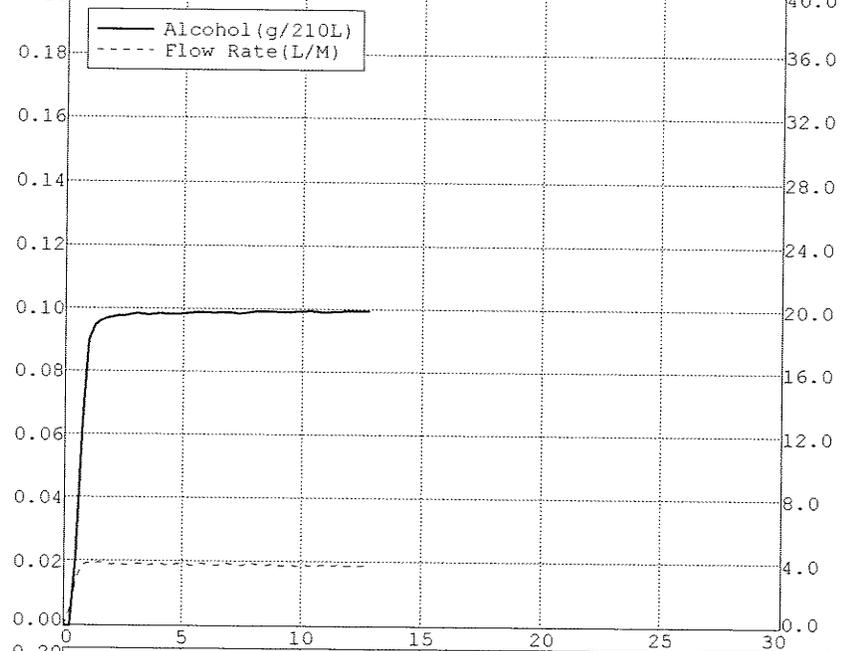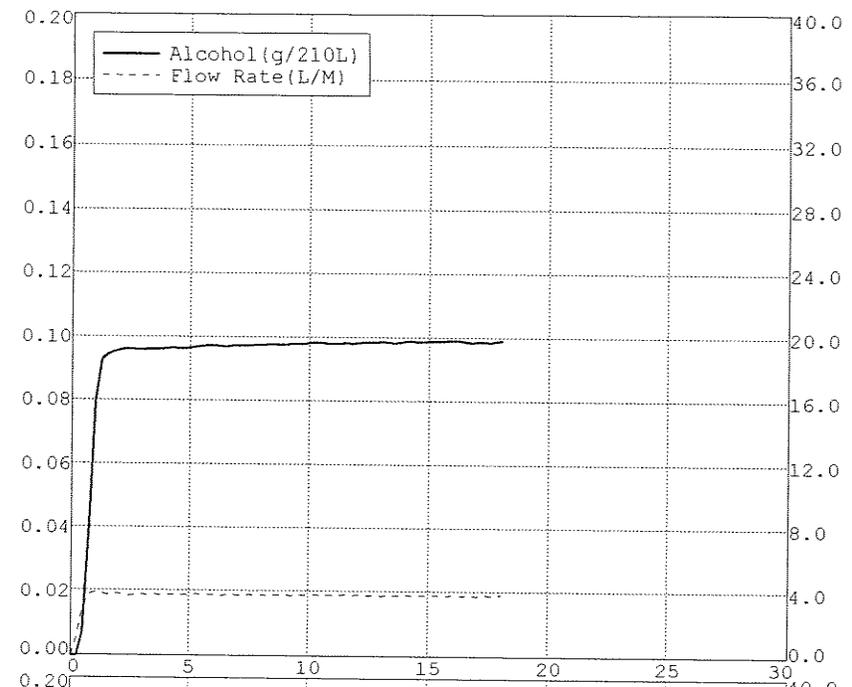

Charles B. Geisler