

SUPERVISOR TEST




WARREN COUNTY  
SHERIFF'S OFFICE  
DATAMASTER dmt: 144506

Date: 05/23/2022

OPERATOR NAME:  
J RIEHL  
Permit #: 47503  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 22030

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:01
INTERNAL STANDARD	VERIFIED	01:01
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	01:02
BLANK TEST	0.00	01:02
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	01:03
BLANK TEST	0.00	01:04
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	01:04
BLANK TEST	0.00	01:05

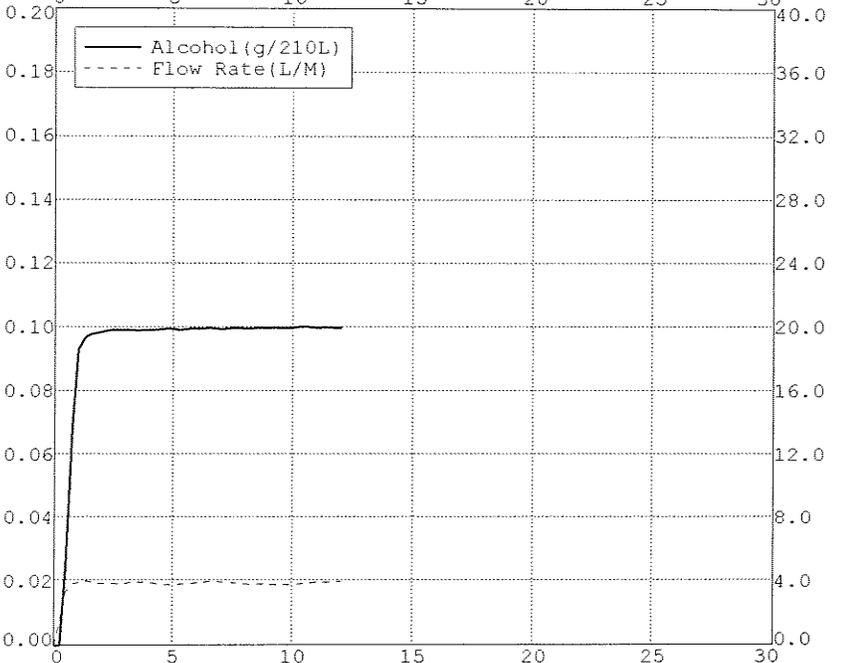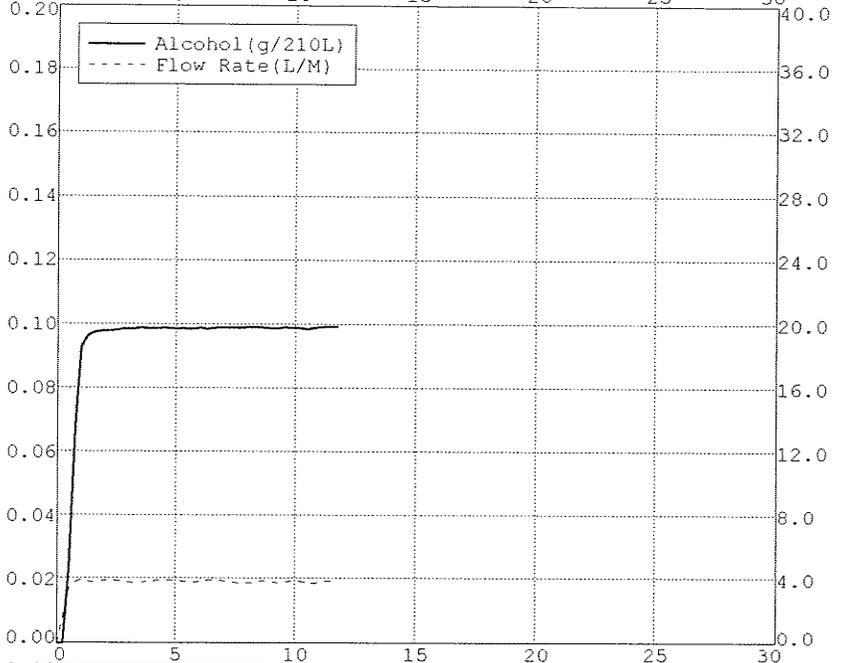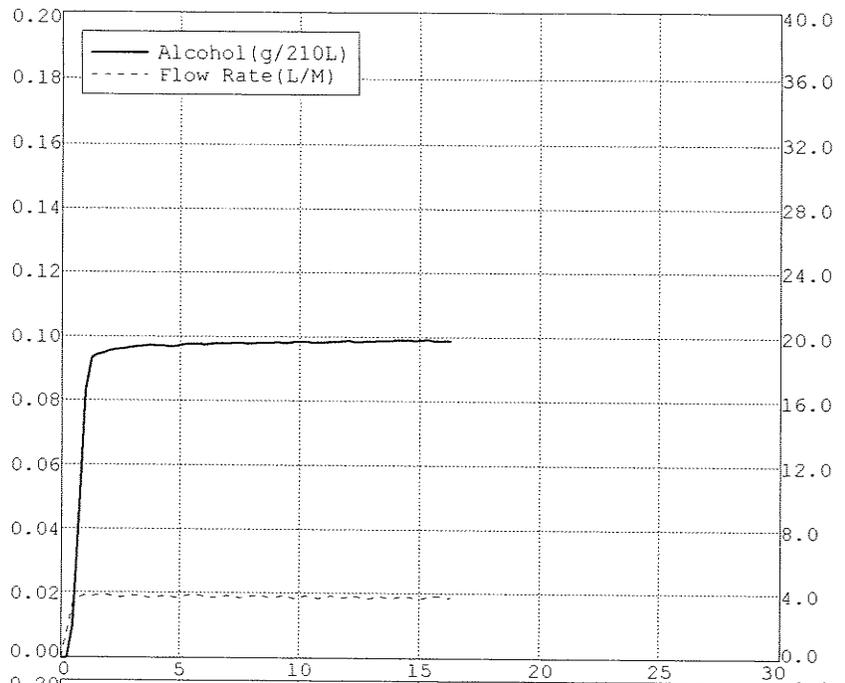

*J Riehl*  
#820