

SUPERVISOR TEST




WARREN COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 08/08/2022

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 22190

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:36
INTERNAL STANDARD	VERIFIED	13:36
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	13:37
BLANK TEST	0.00	13:38
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	13:38
BLANK TEST	0.00	13:39
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	13:39
BLANK TEST	0.00	13:40

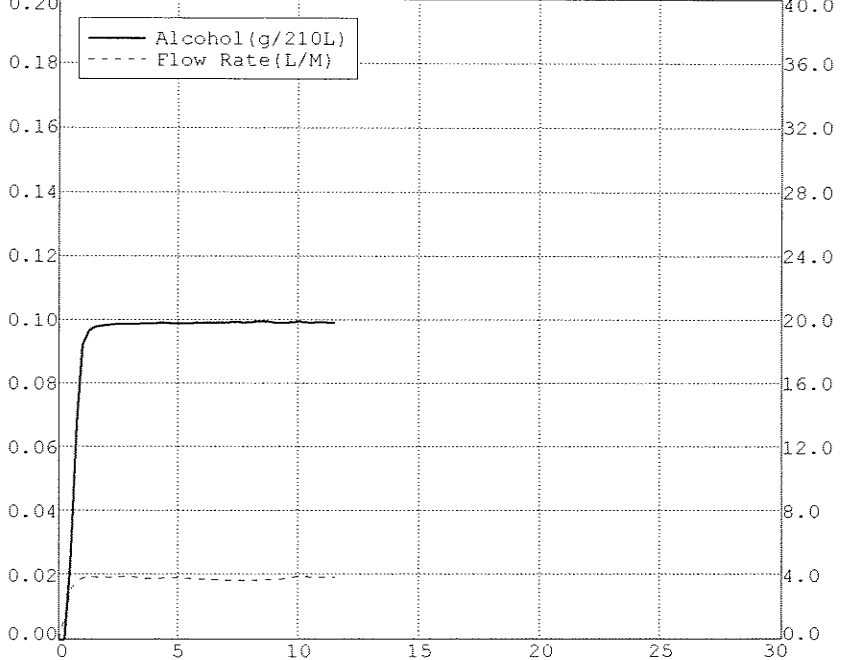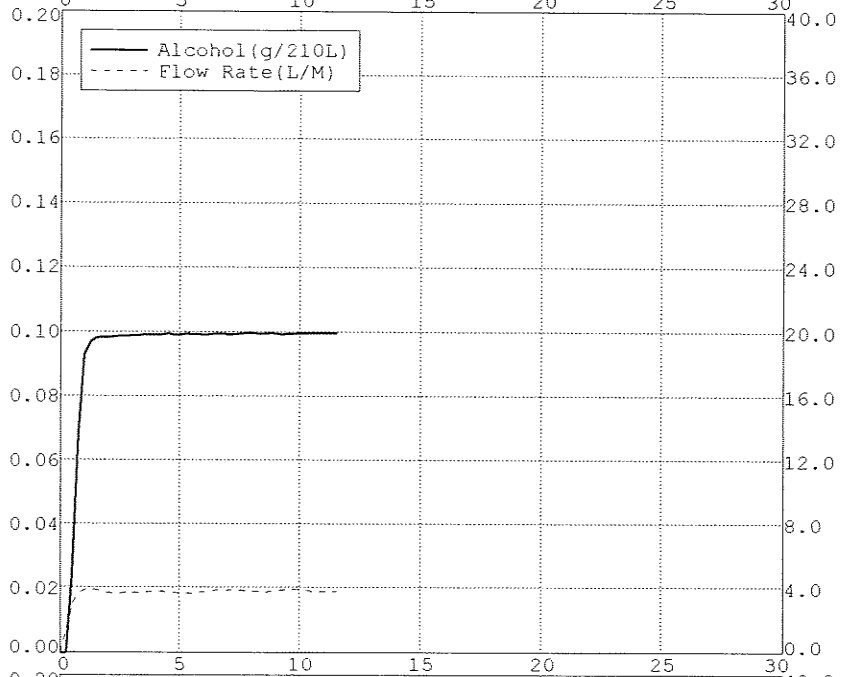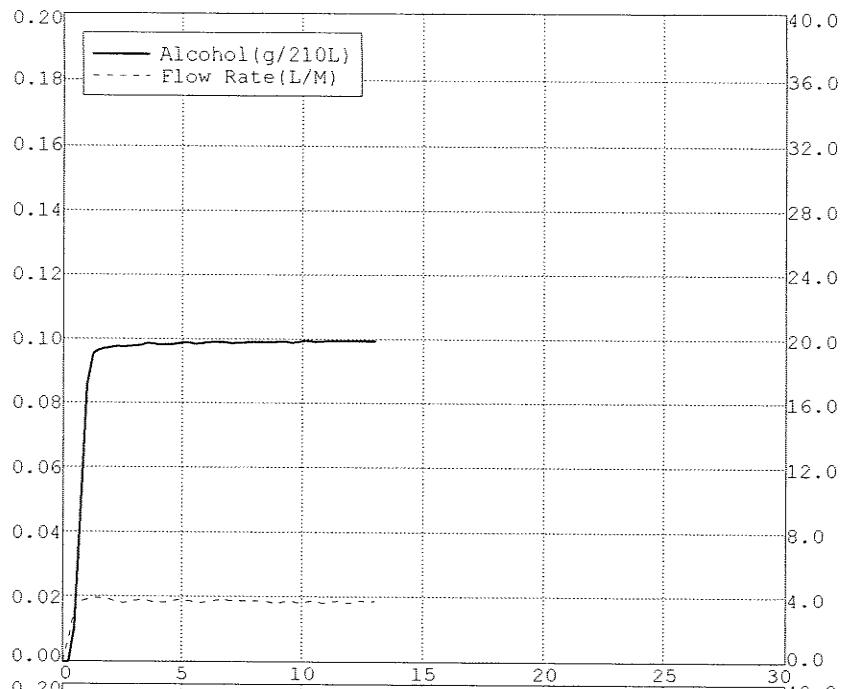

Handwritten signature and initials: J. H. S. [Signature] #211