

SOLUTION CHANGE

-----  
WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208  
-----



Date: 12/01/2022

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 22390

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:59
INTERNAL STANDARD	VERIFIED	12:59
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	12:59
BLANK TEST	0.00	13:00
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	13:00

Blank Error

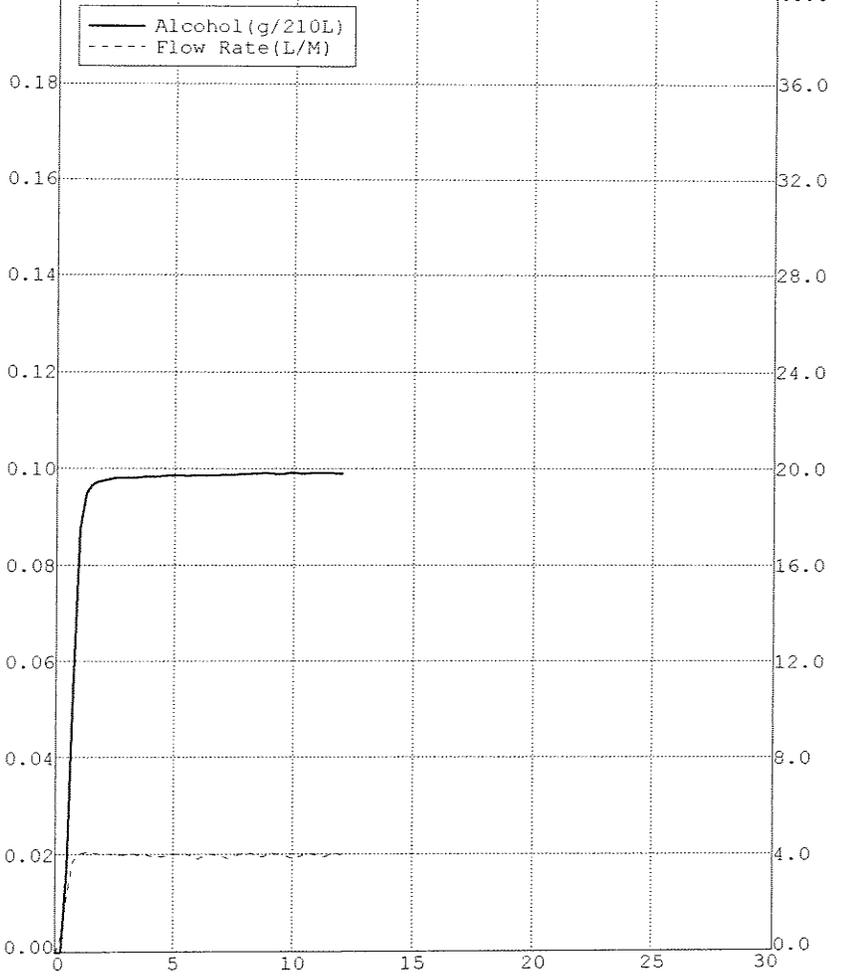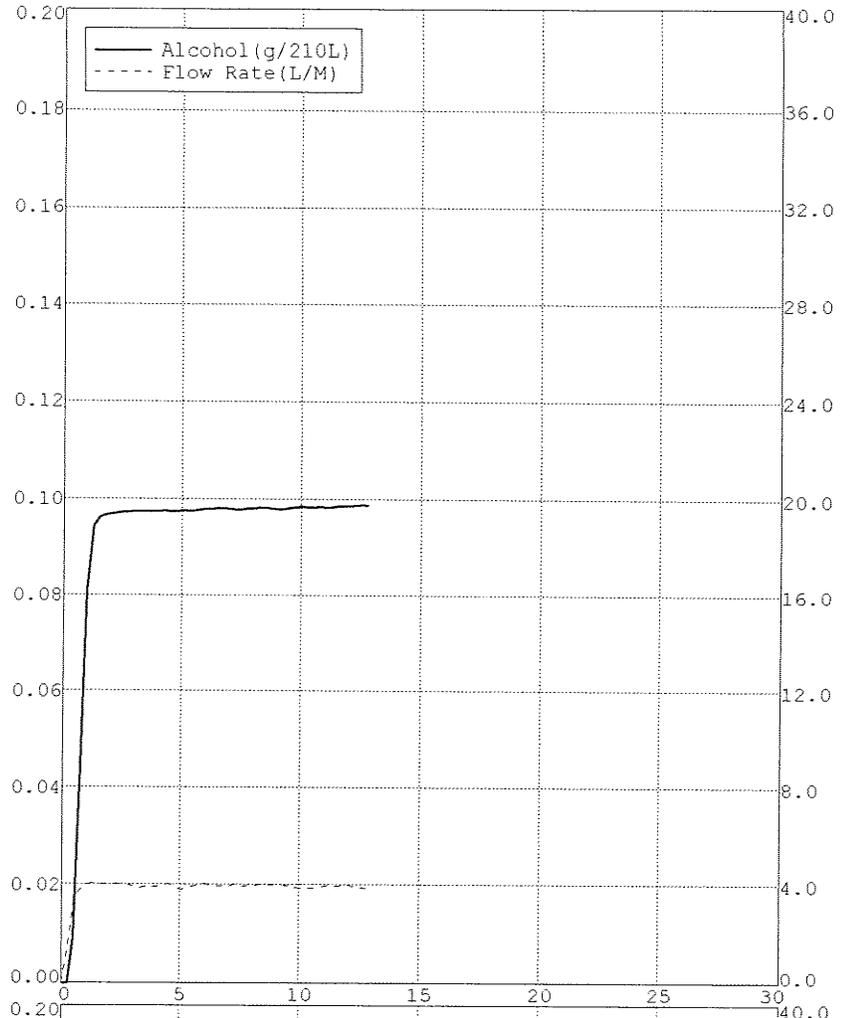

*Charles B. Geisler*

SOLUTION CHANGE




WARREN COUNTY  
 SHERIFF'S OFFICE  
 DATAMASTER dmt: 144506

Date: 12/01/2022

OPERATOR NAME:  
 CHARLES B GEISLER  
 Permit #: 33757  
 Operator Agency/Dept: WARREN CO. SO  
 Reference Standard #: 22390

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:58
INTERNAL STANDARD	VERIFIED	13:58
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	13:58
BLANK TEST	0.00	13:59
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	13:59
BLANK TEST	0.00	14:00
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	14:00
BLANK TEST	0.00	14:01

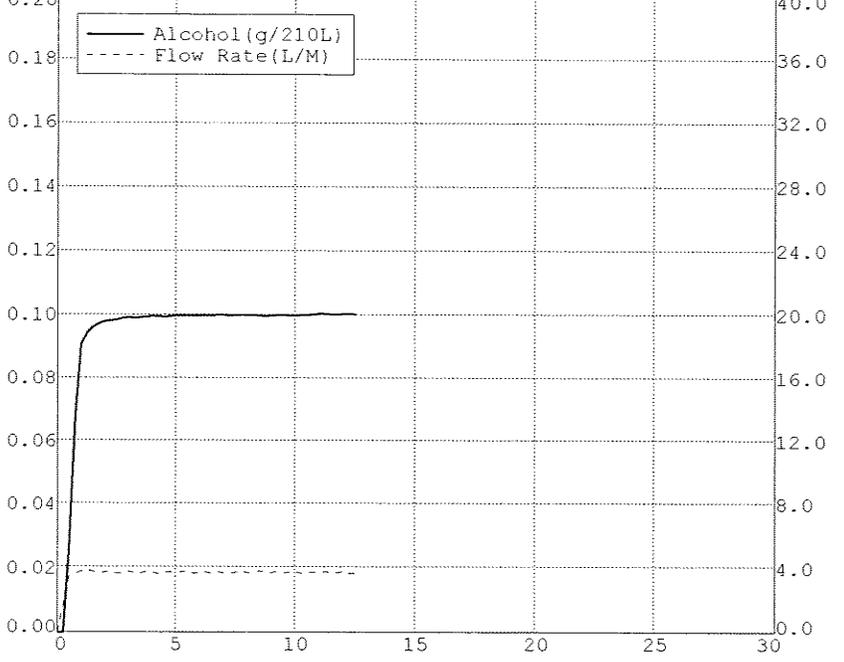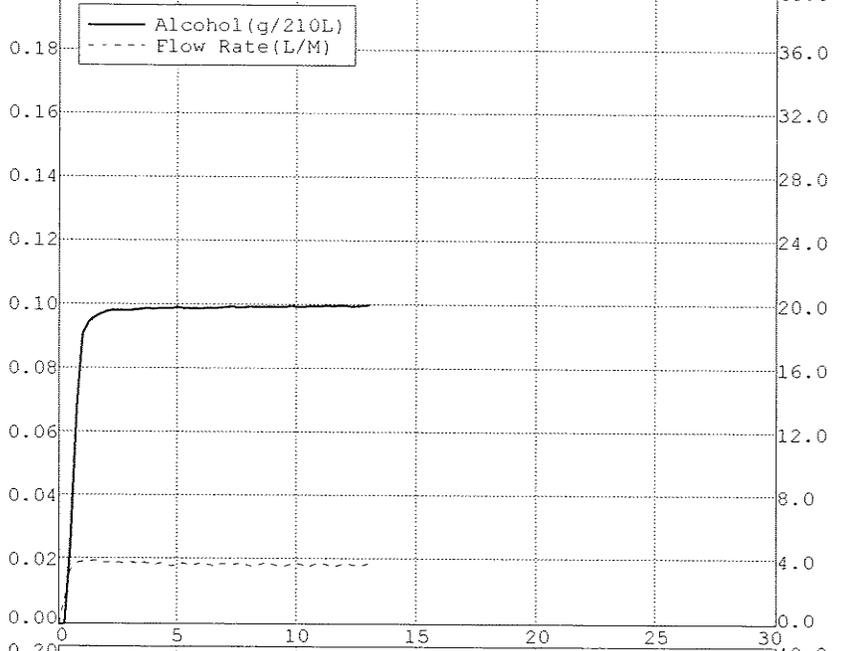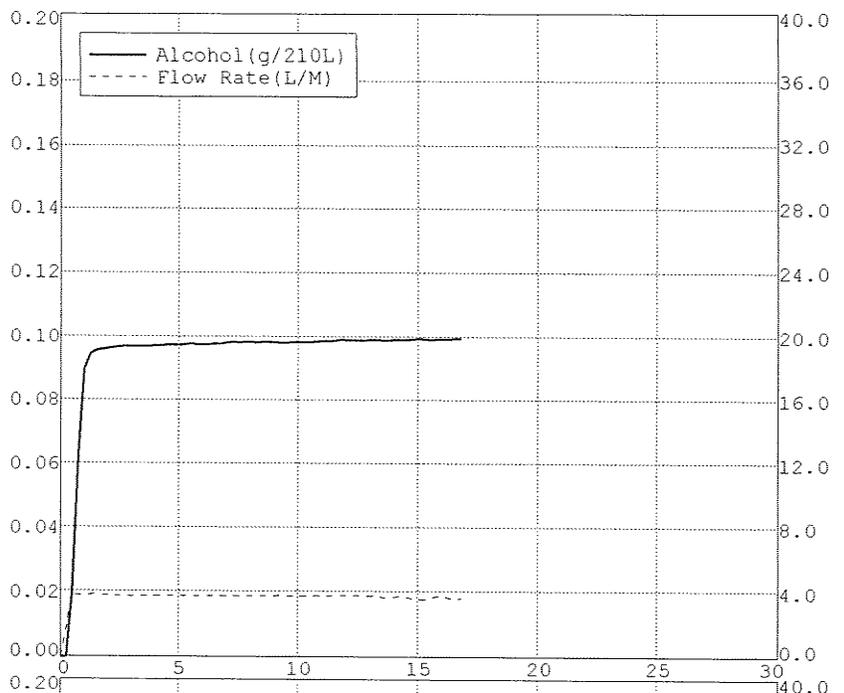

*Handwritten signature and initials*

SOLUTION CHANGE




-----  
 WARREN CO.  
 SHERIFF'S OFFICE  
 DATAMASTER dmt: 105208  
 -----

Date: 12/01/2022

OPERATOR NAME:  
 CHARLES B GEISLER  
 Permit #: 33757  
 Operator Agency/Dept: WARREN CO. SO  
 Reference Standard #: 22390

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:06
INTERNAL STANDARD	VERIFIED	13:06
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.00	13:06
BLANK TEST	0.00	13:07
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.00	13:07
BLANK TEST	0.00	13:08
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.00	13:09
BLANK TEST	0.00	13:09

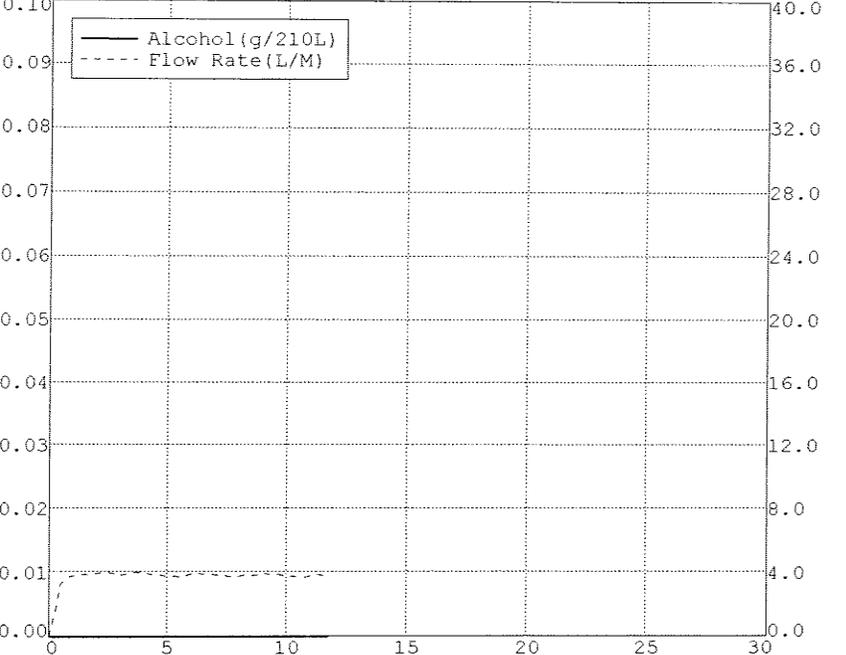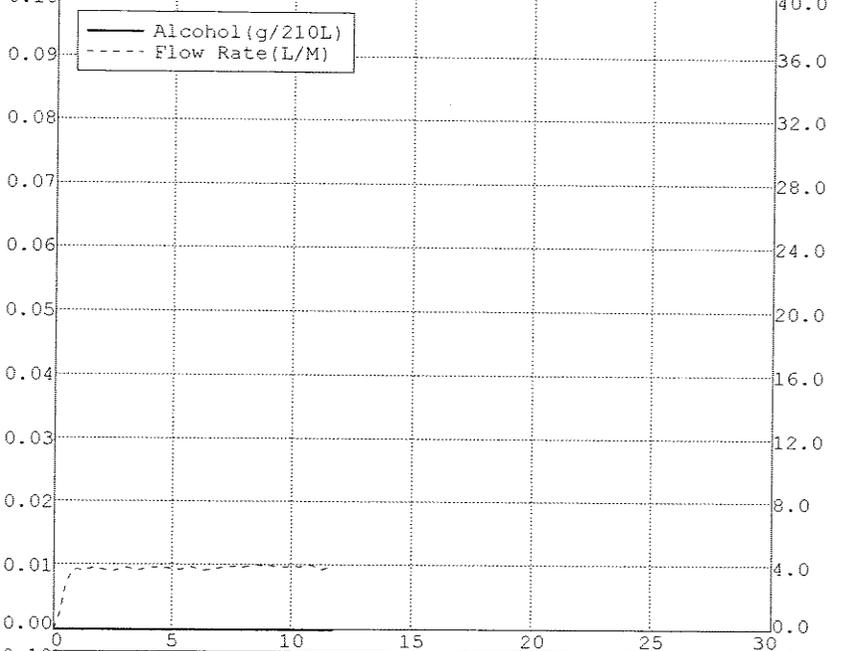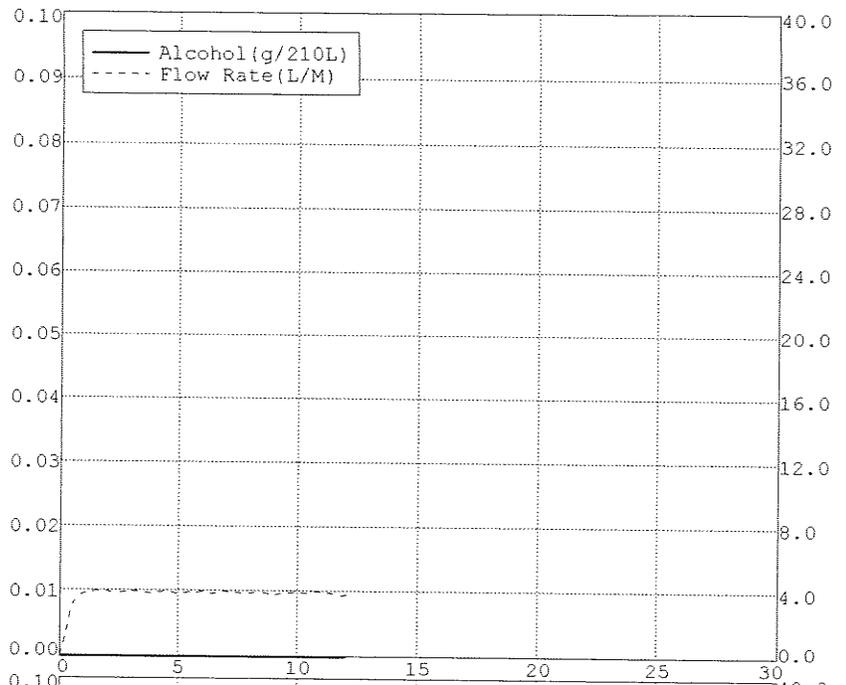

*Sgt. Charles B. Geisler*