

SUPERVISOR TEST




WARREN COUNTY  
SHERIFF'S OFFICE  
DATAMASTER dmt: 144506

Date: 12/26/2022

OPERATOR NAME:  
SEAN T SMITH  
Permit #: 46227  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 22390

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:37
INTERNAL STANDARD	VERIFIED	09:37
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	09:38
BLANK TEST	0.00	09:39
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	09:39
BLANK TEST	0.00	09:40
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	09:40
BLANK TEST	0.00	09:41

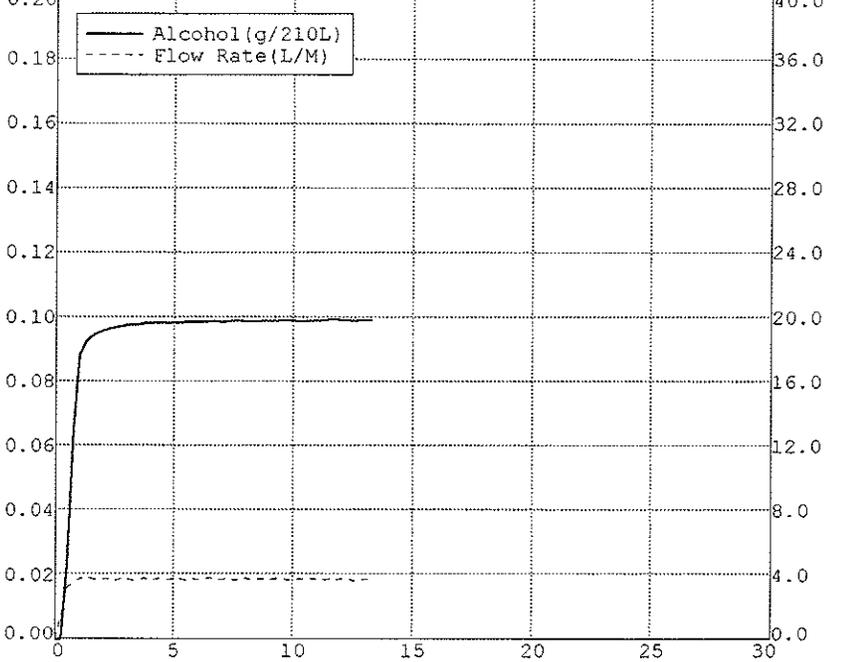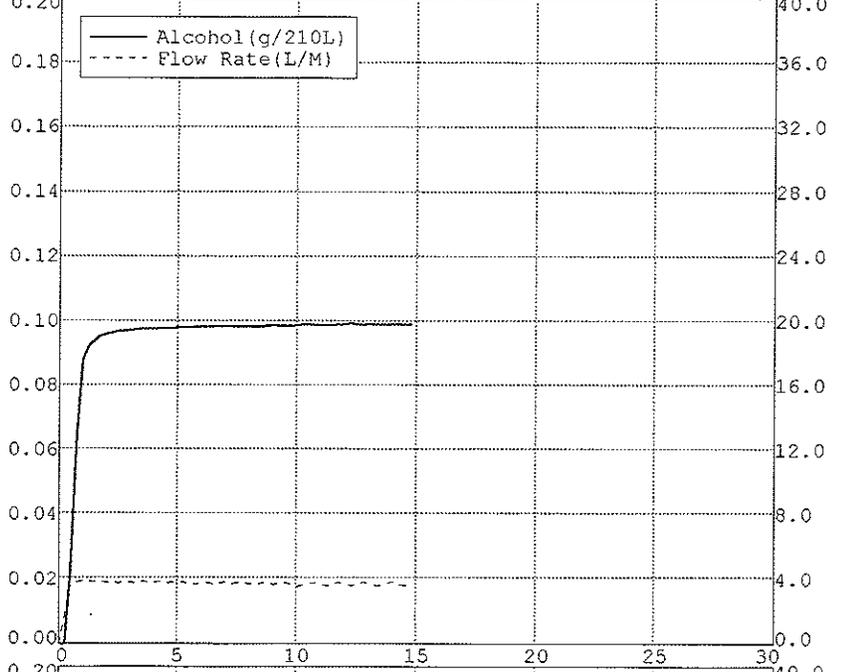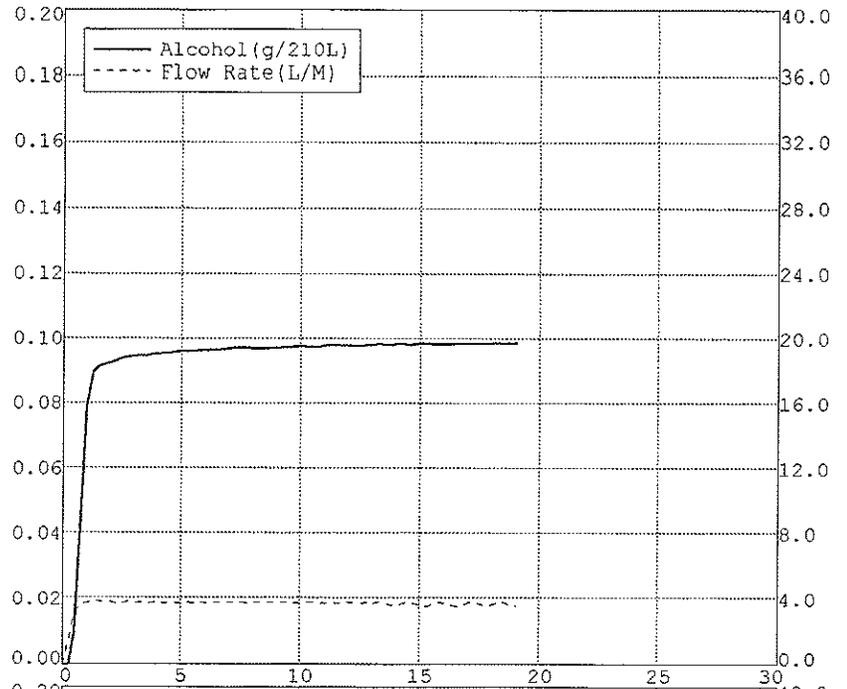

*Handwritten signature and initials*