

SOLUTION CHANGE




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 03/31/2023

OPERATOR NAME:
MICHAEL A CAMPBELL
Permit #: 42422
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 23030

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:32
INTERNAL STANDARD	VERIFIED	00:32
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	00:32
BLANK TEST	0.00	00:33
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	00:33
BLANK TEST	0.00	00:34
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	00:34
BLANK TEST	0.00	00:35

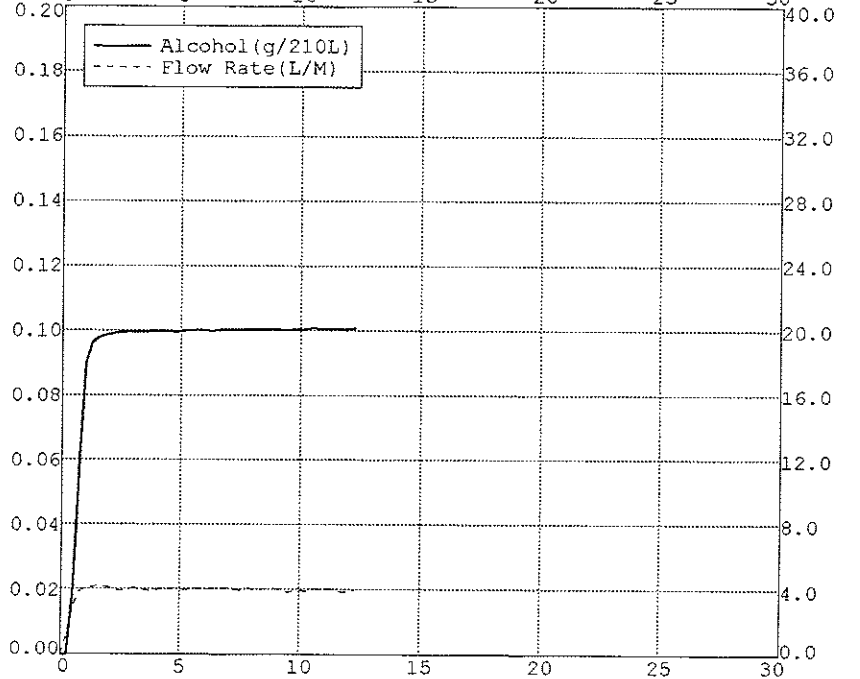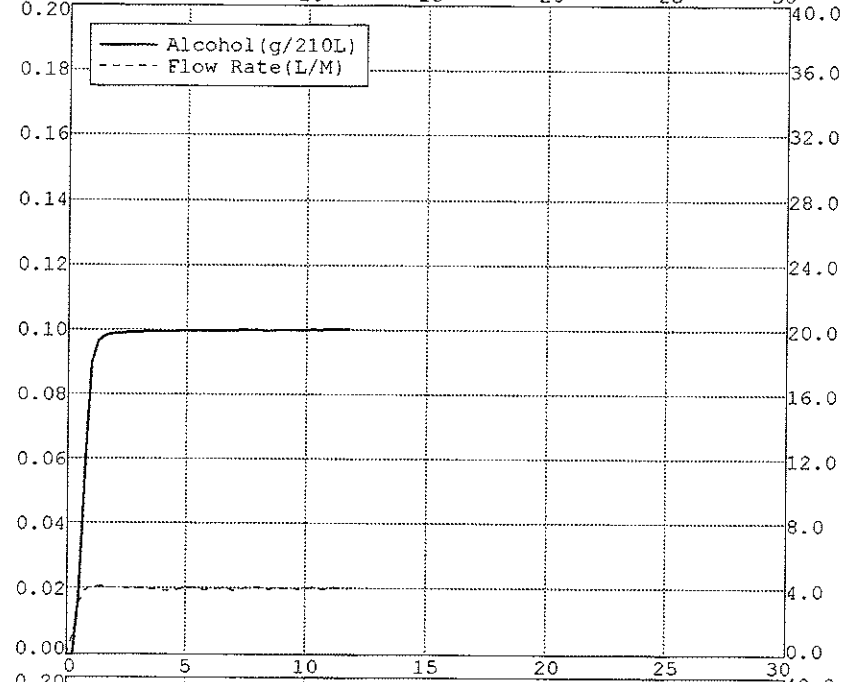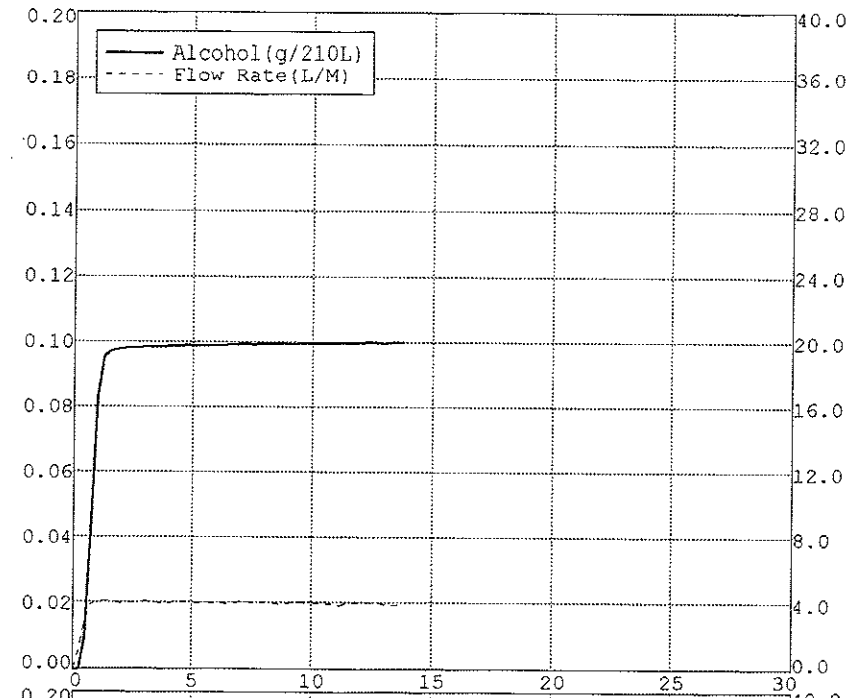

[Handwritten signature] #757