

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 05/15/2023

OPERATOR NAME:
SEAN T SMITH
Permit #: 46227
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 23030

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:26
INTERNAL STANDARD	VERIFIED	09:26
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	09:26
BLANK TEST	0.00	09:27
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	09:28
BLANK TEST	0.00	09:28
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	09:29
BLANK TEST	0.00	09:30

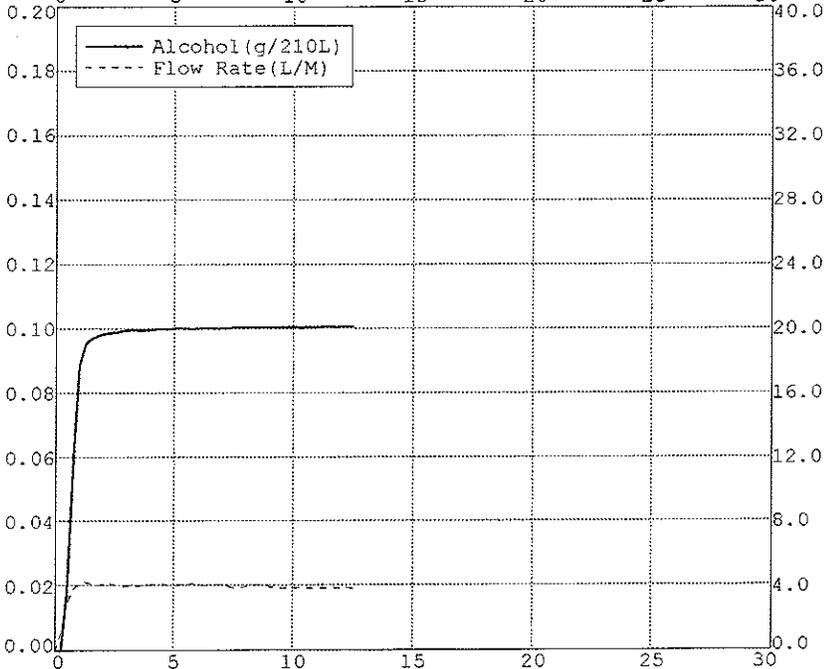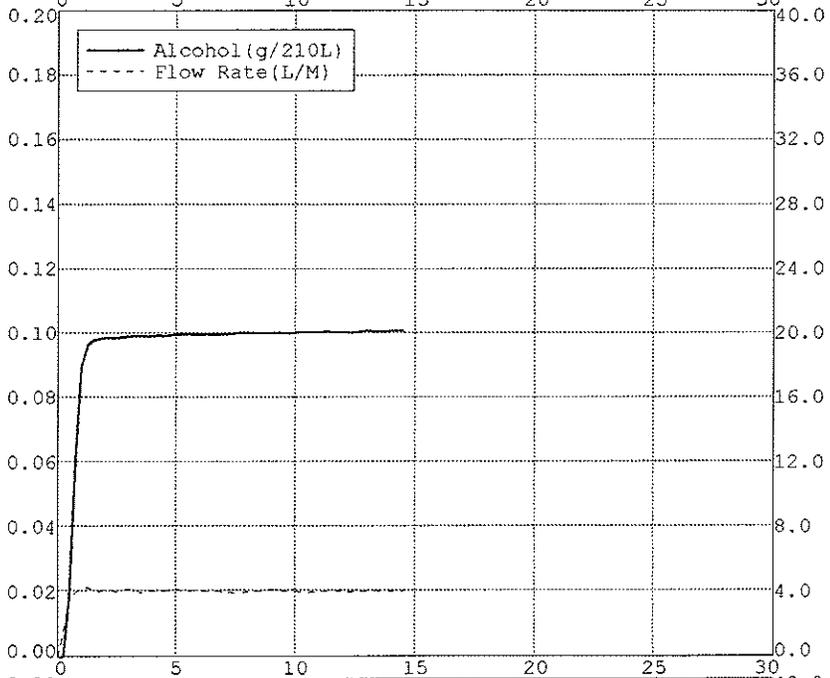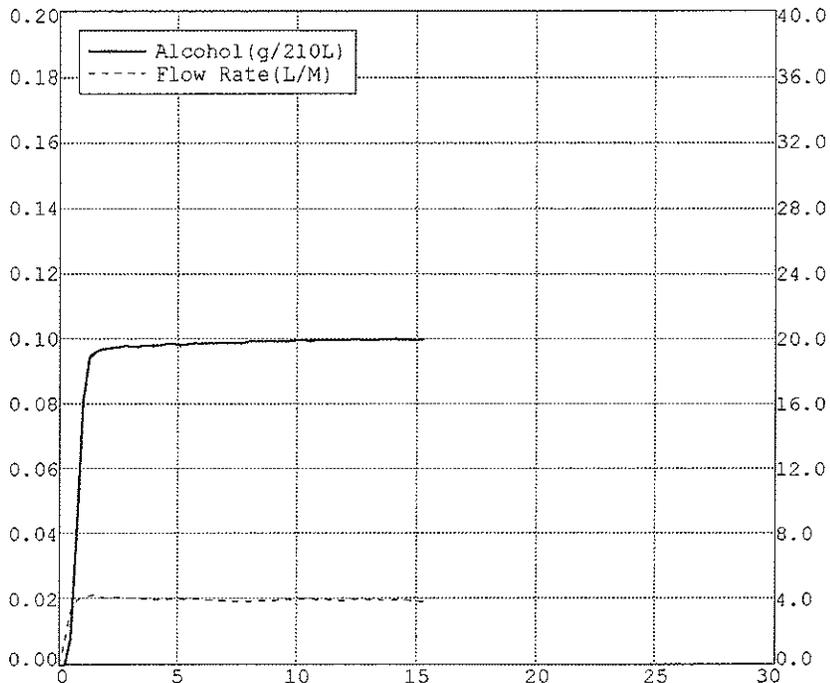

ST 85