

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 06/16/2023

OPERATOR NAME:  
SEAN T SMITH  
Permit #: 46227  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 23090

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:19
INTERNAL STANDARD	VERIFIED	16:20
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:20
BLANK TEST	0.00	16:21
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:21
BLANK TEST	0.00	16:22
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:22
BLANK TEST	0.00	16:23

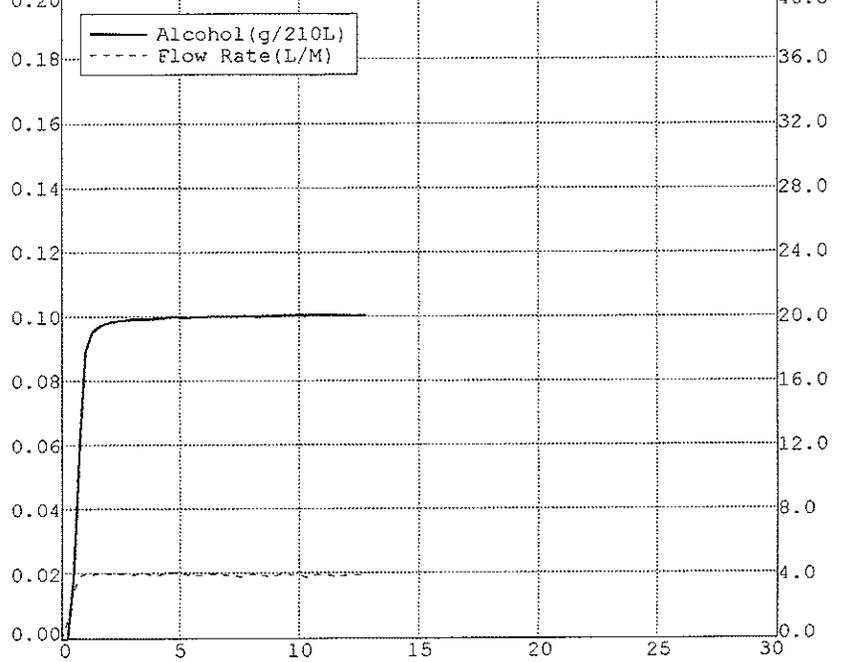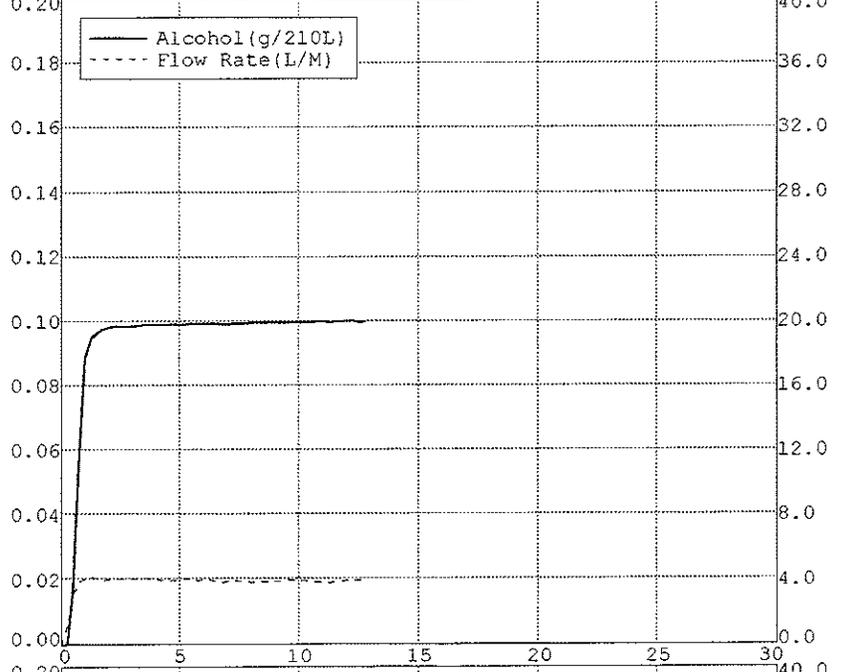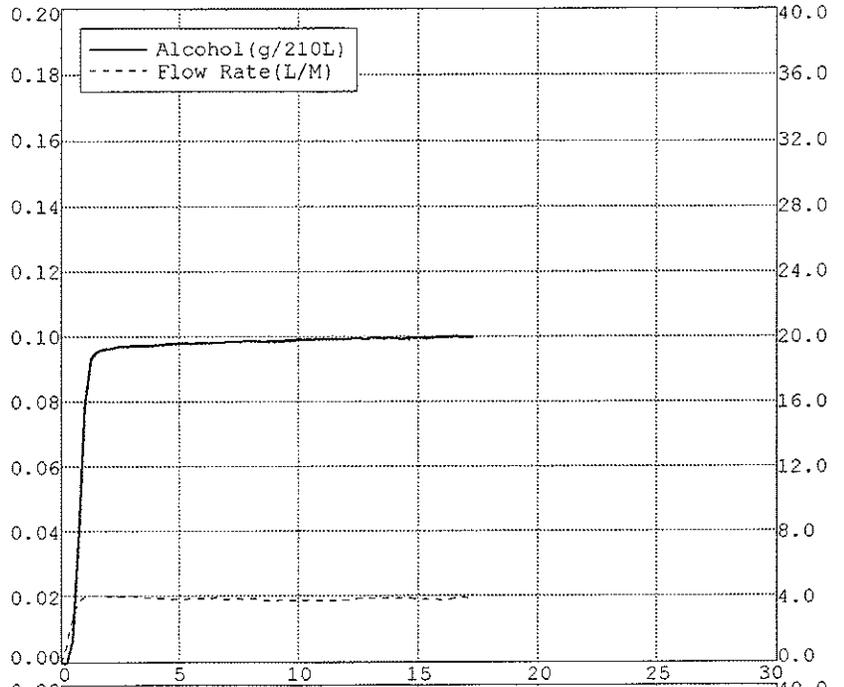

*Signature* 8/5