

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 11/22/2023

OPERATOR NAME:
JOHN D BATEHOLTS
Permit #: 43007
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 23270

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:27
INTERNAL STANDARD	VERIFIED	10:27
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	10:28
BLANK TEST	0.00	10:29
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	10:29
BLANK TEST	0.00	10:30
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	10:30
BLANK TEST	0.00	10:31

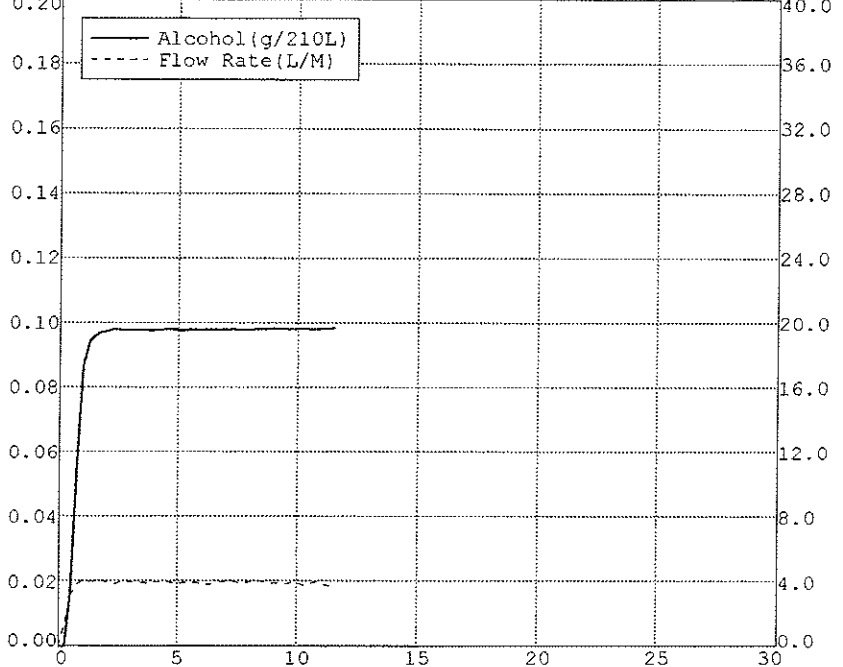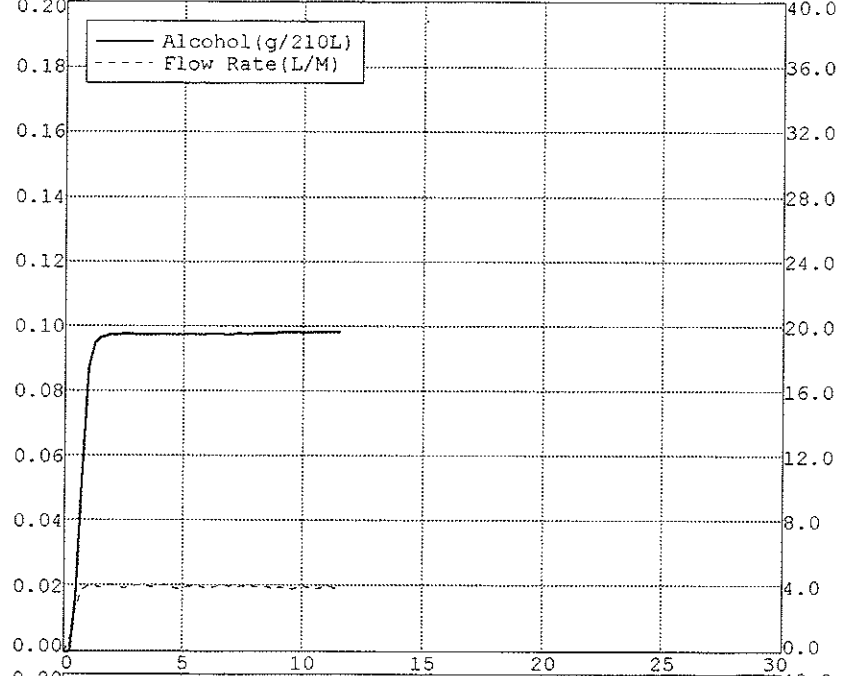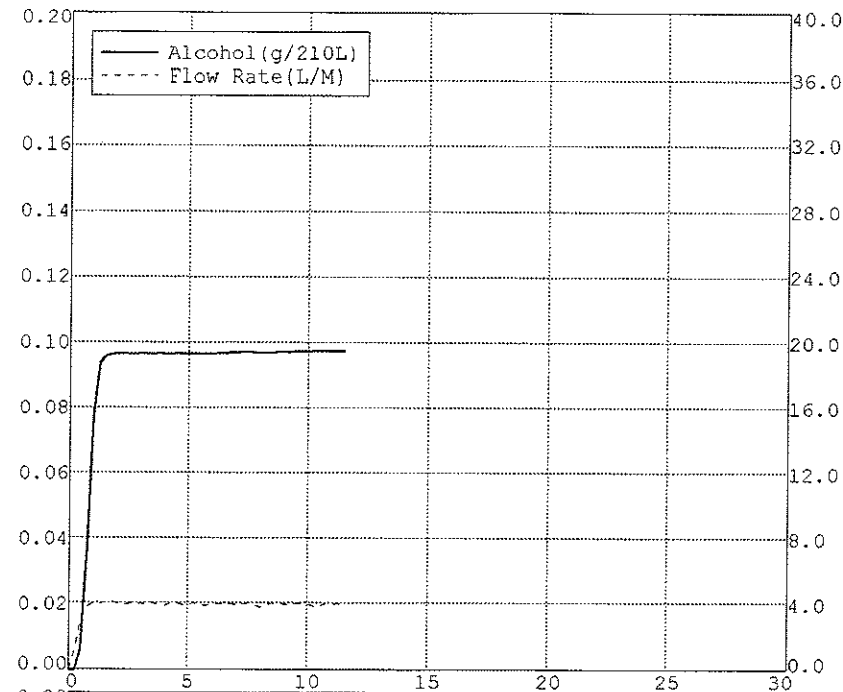

John D Bateholts 11/22/23