

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 02/03/2023

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 22420

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:21
INTERNAL STANDARD	VERIFIED	10:21
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	10:22
BLANK TEST	0.00	10:22
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	10:23
BLANK TEST	0.00	10:24
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	10:24
BLANK TEST	0.00	10:25

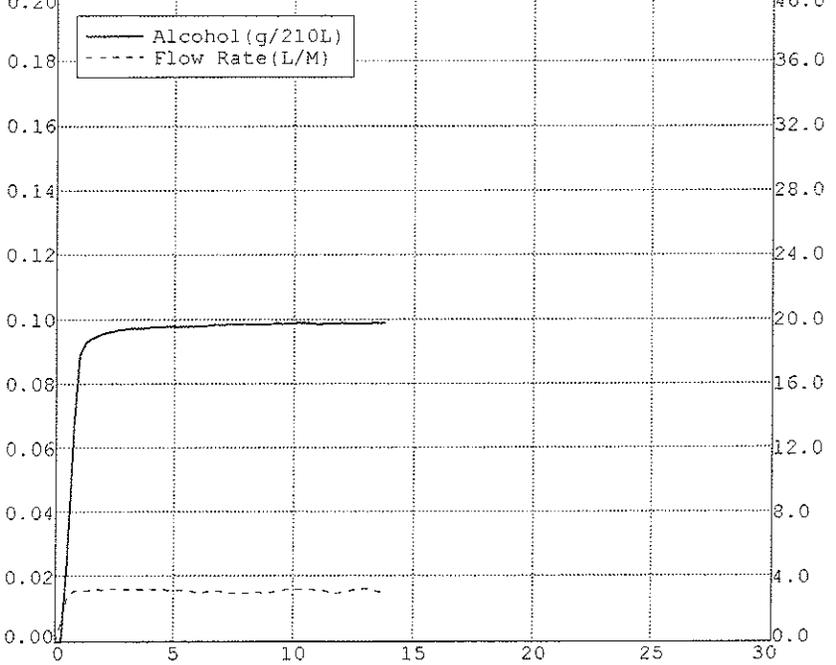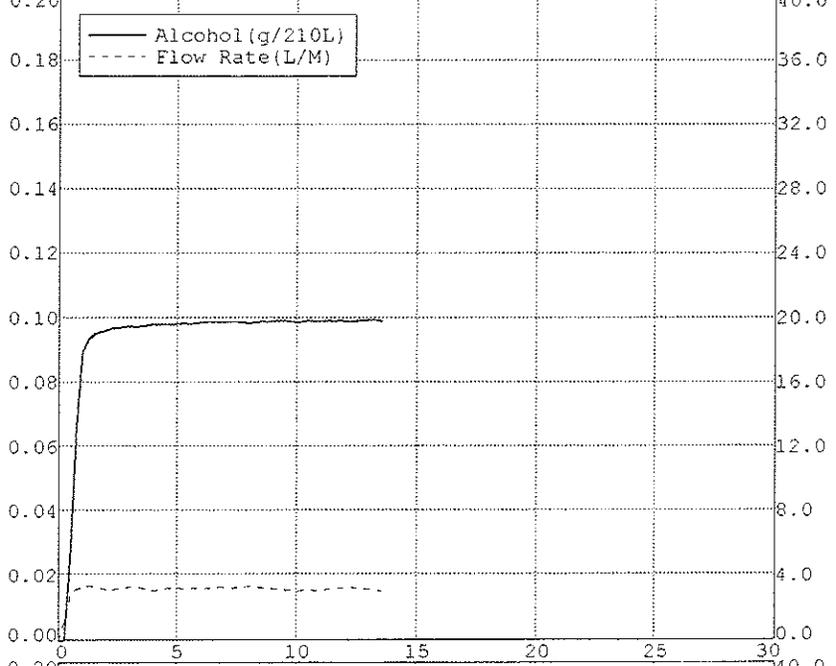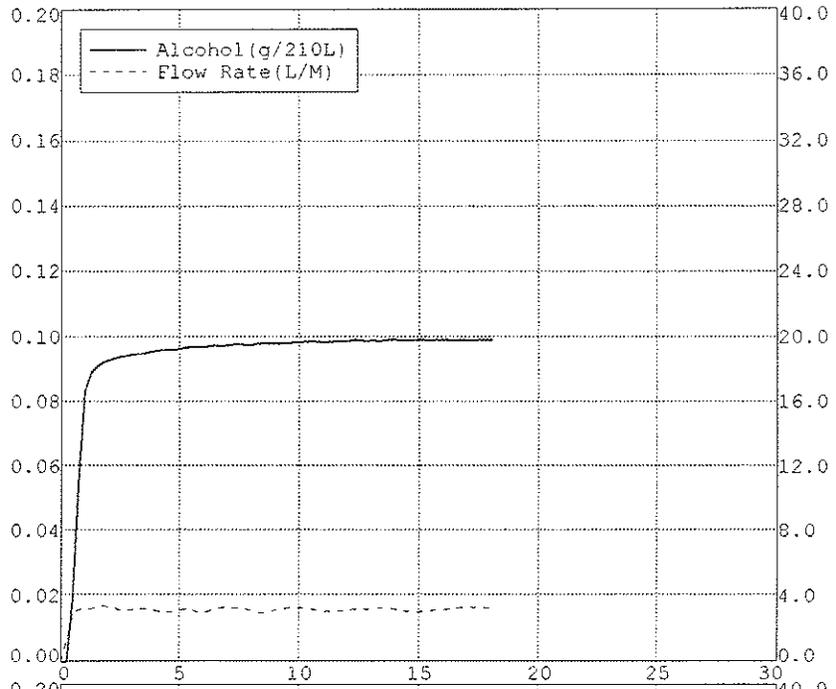

Charles B. Geisler #244