

SUPERVISOR TEST


WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 02/15/2023

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 22420

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:12
INTERNAL STANDARD	VERIFIED	13:12
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	13:13
BLANK TEST	0.00	13:14
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	13:14
BLANK TEST	0.00	13:15
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	13:15
BLANK TEST	0.00	13:16

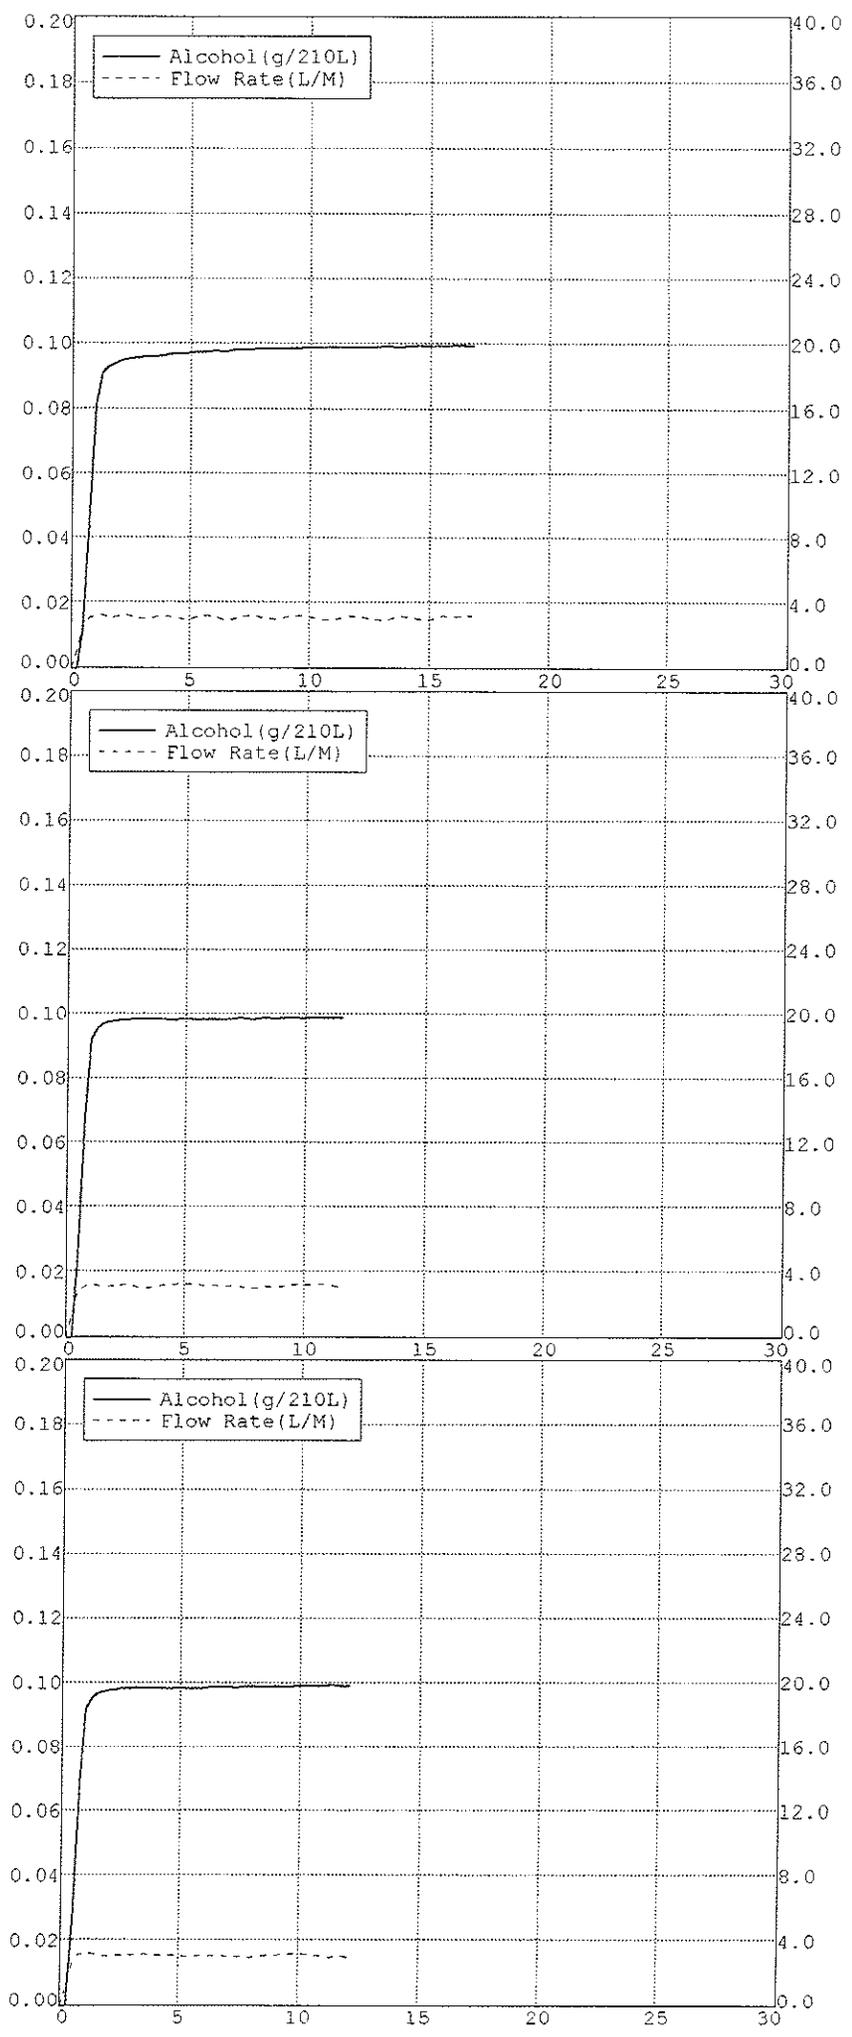

Charles B Geisler
#241