

SOLUTION CHANGE




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 03/31/2023

OPERATOR NAME:
MICHAEL A CAMPBELL
Permit #: 42422
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 23030

Nominal = 0.10 g/210L

BLANK TEST	0.00	06:44
INTERNAL STANDARD	VERIFIED	06:44
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	06:45
BLANK TEST	0.00	06:46
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	06:46
BLANK TEST	0.00	06:47
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	06:47
BLANK TEST	0.00	06:48

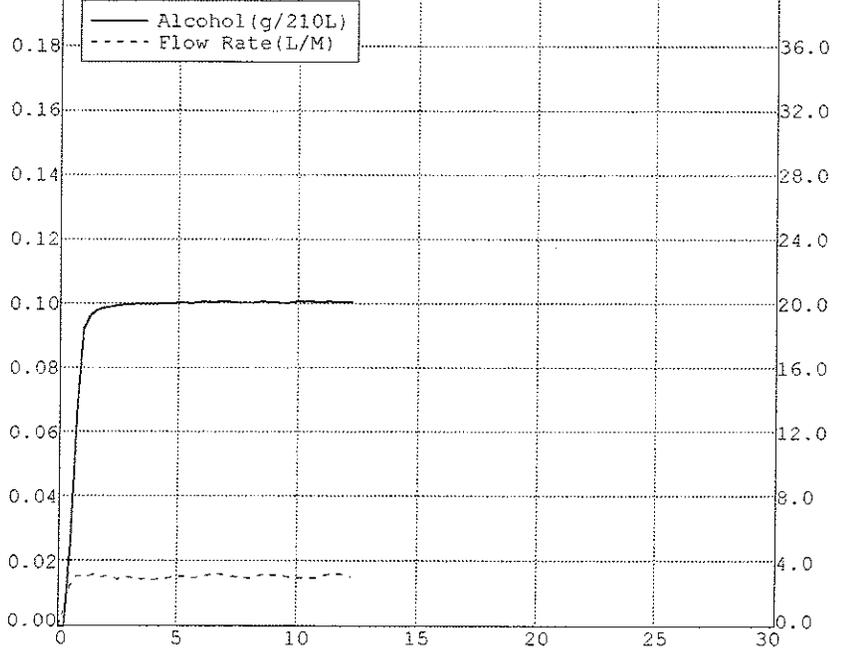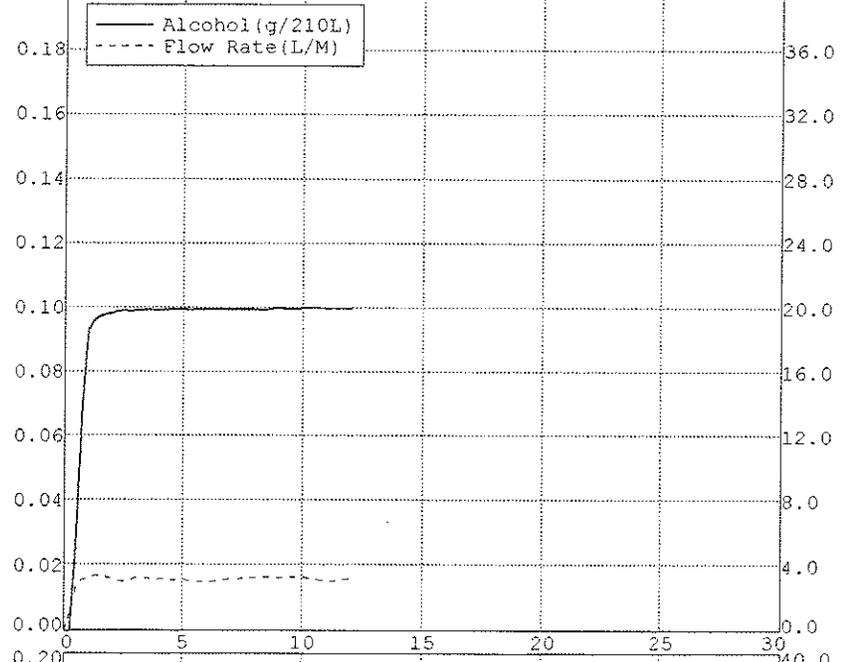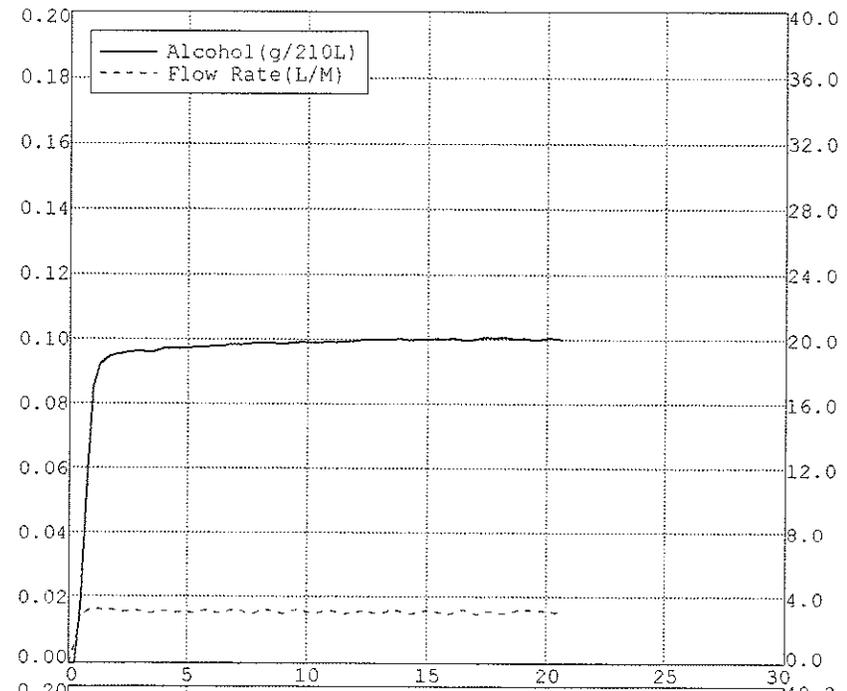

Michael A Campbell #1157