

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 05/15/2023

OPERATOR NAME:
SEAN T SMITH
Permit #: 46227
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 23030

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:10
INTERNAL STANDARD	VERIFIED	08:11
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	08:11
BLANK TEST	0.00	08:12
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	08:12
BLANK TEST	0.00	08:13
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	08:13
BLANK TEST	0.00	08:14

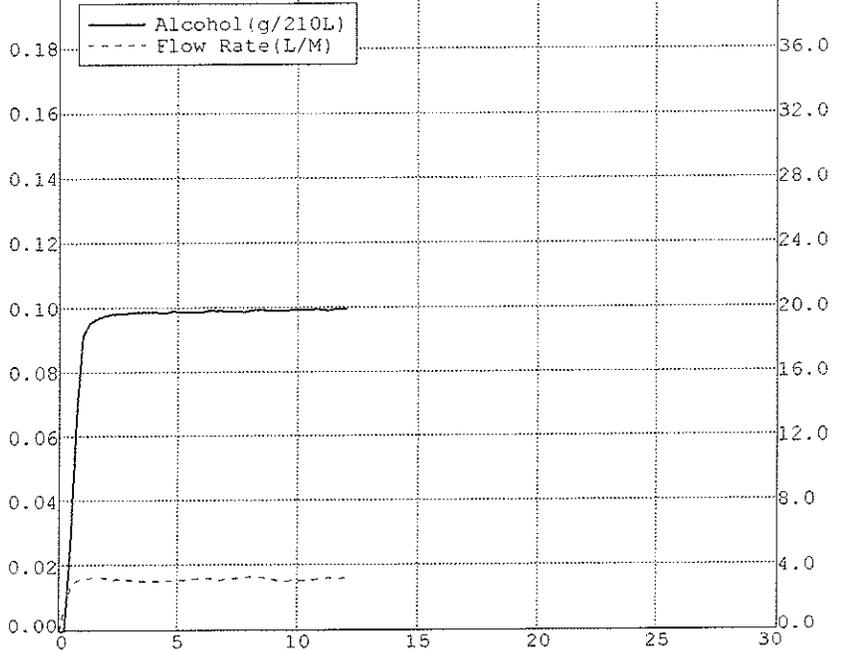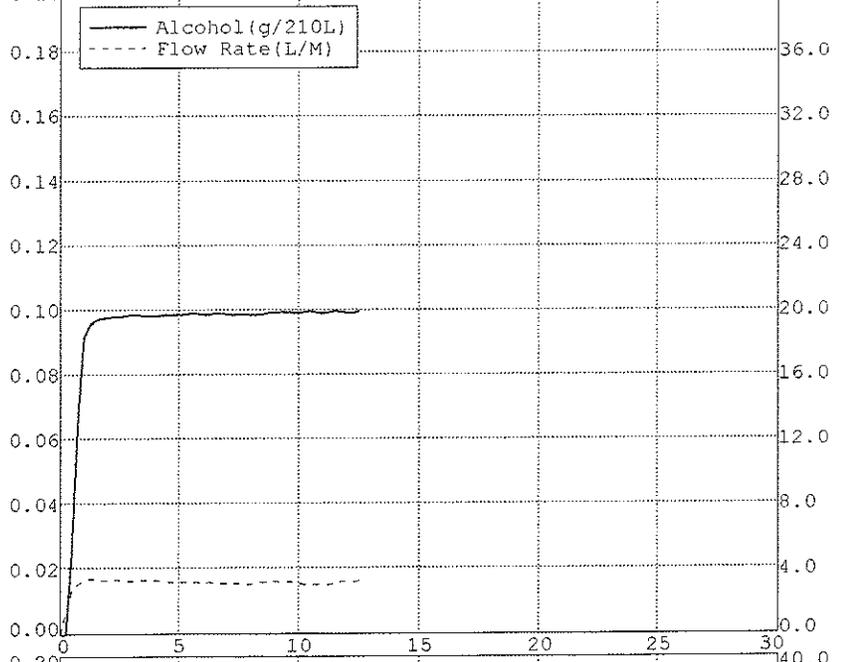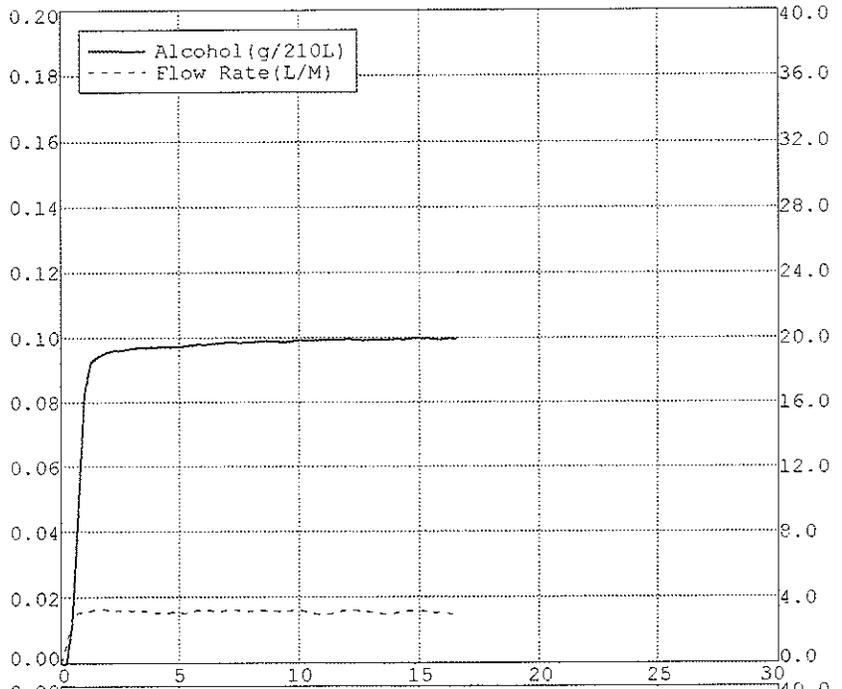

Handwritten signature and initials