

SOLUTION CHANGE




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 06/02/2023

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 23090

Nominal = 0.10 g/210L

|                         |          |       |
|-------------------------|----------|-------|
| BLANK TEST              | 0.00     | 10:04 |
| INTERNAL STANDARD       | VERIFIED | 10:04 |
| REFERENCE STANDARD TEMP | 34.01c   |       |
| REFERENCE STANDARD      | 0.10     | 10:04 |
| BLANK TEST              | 0.00     | 10:05 |
| REFERENCE STANDARD TEMP | 34.02c   |       |
| REFERENCE STANDARD      | 0.10     | 10:06 |
| BLANK TEST              | 0.00     | 10:06 |
| REFERENCE STANDARD TEMP | 34.02c   |       |
| REFERENCE STANDARD      | 0.10     | 10:07 |
| BLANK TEST              | 0.00     | 10:08 |

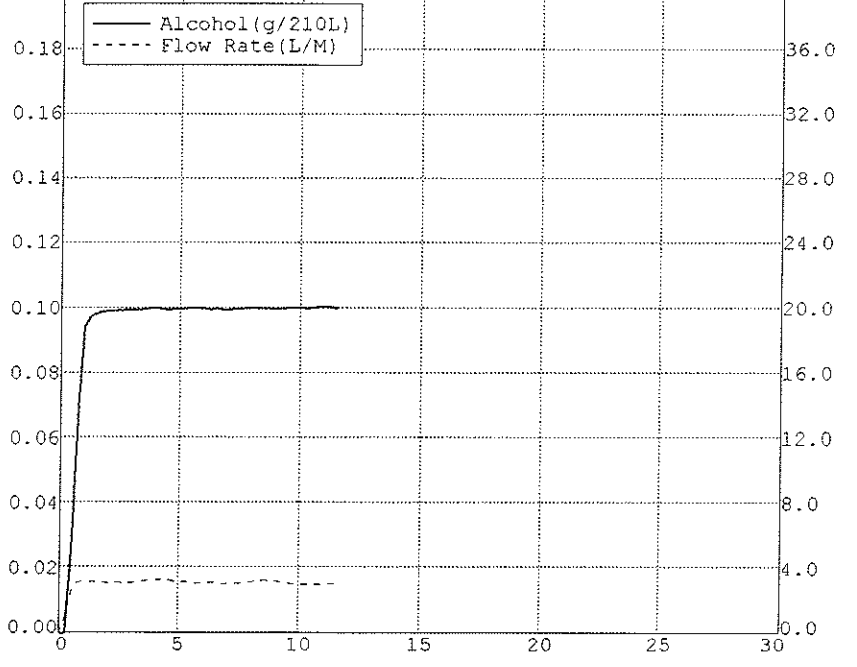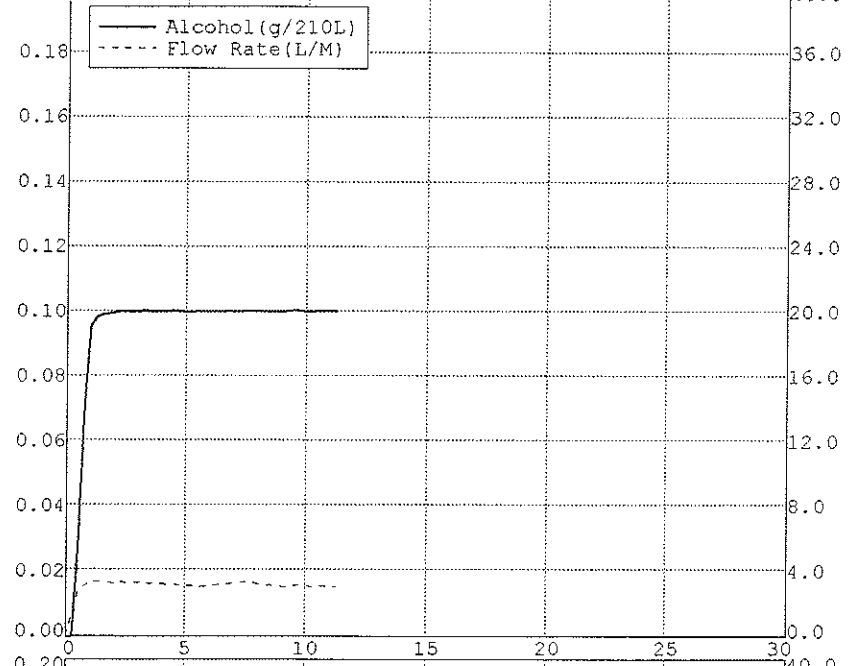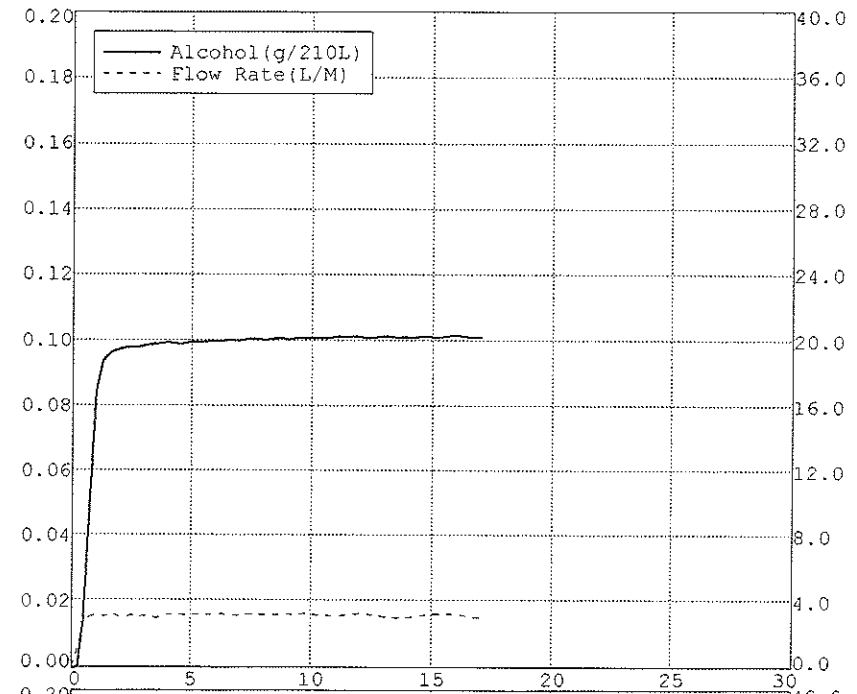

*Signature: C. B. Geisler*