

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 07/16/2023

OPERATOR NAME:
JOHN D BATEHOLTS
Permit #: 43007
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 23090

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:02
INTERNAL STANDARD	VERIFIED	08:02
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	08:02
BLANK TEST	0.00	08:03
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	08:03
BLANK TEST	0.00	08:04
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	08:04
BLANK TEST	0.00	08:05

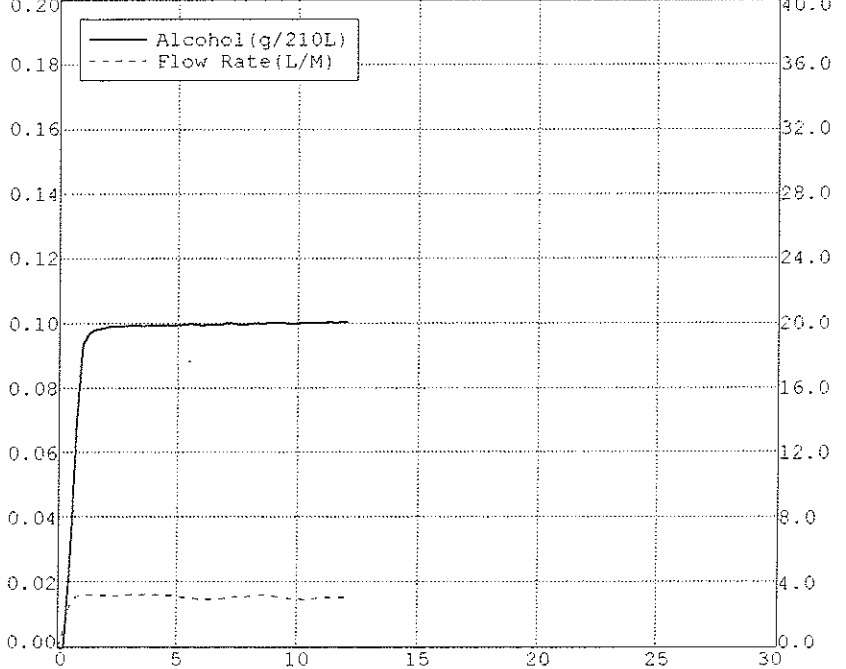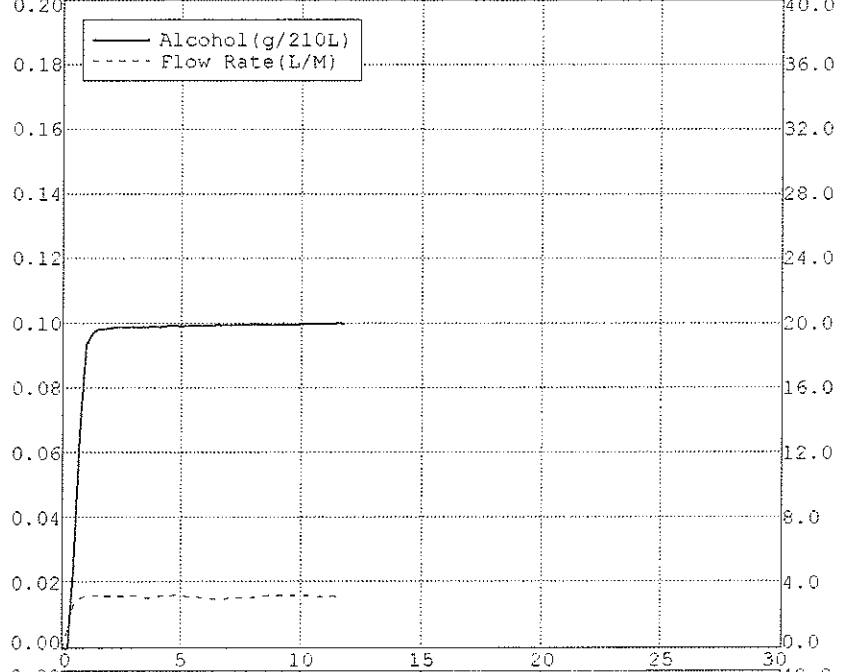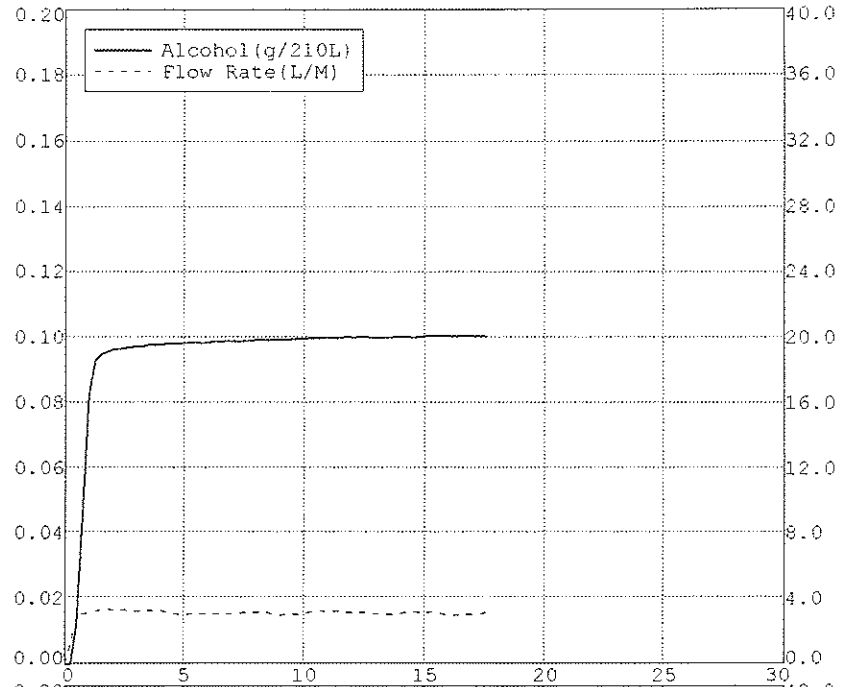

P. J. M. 0714