

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 12/29/2023

OPERATOR NAME:  
JOHN D BATEHOLTS  
Permit #: 43007  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 23350

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:17
INTERNAL STANDARD	VERIFIED	08:17
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	08:17
BLANK TEST	0.00	08:18
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	08:19
BLANK TEST	0.00	08:19
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	08:20
BLANK TEST	0.00	08:21

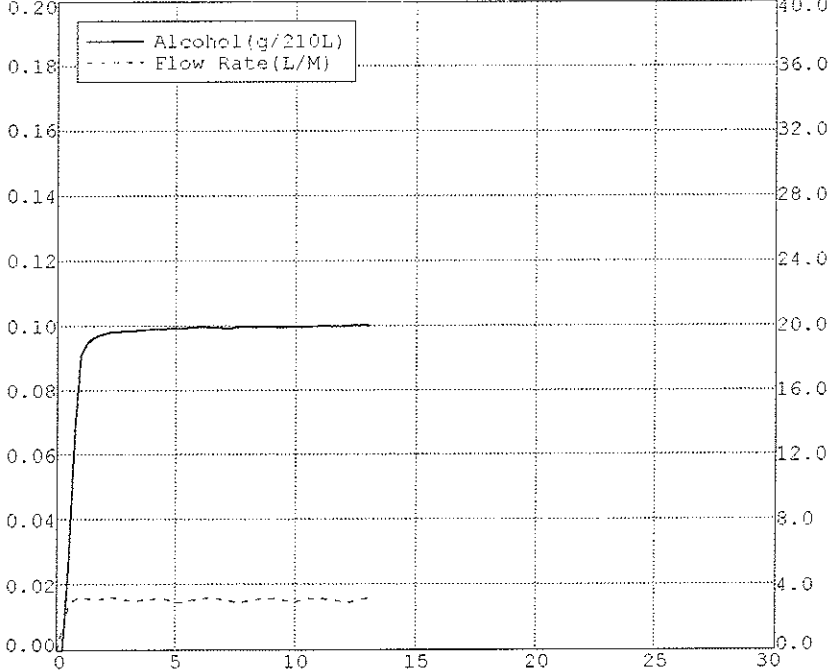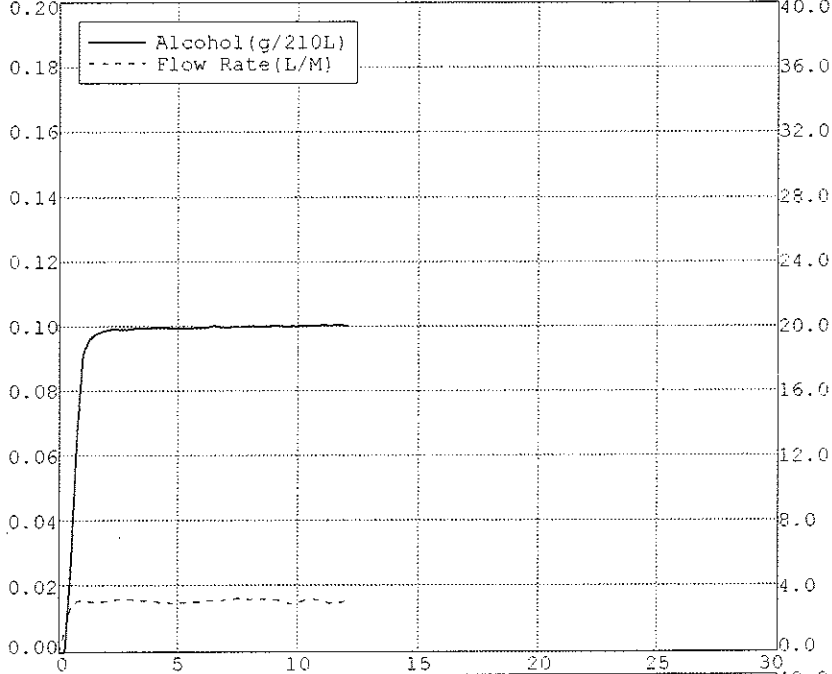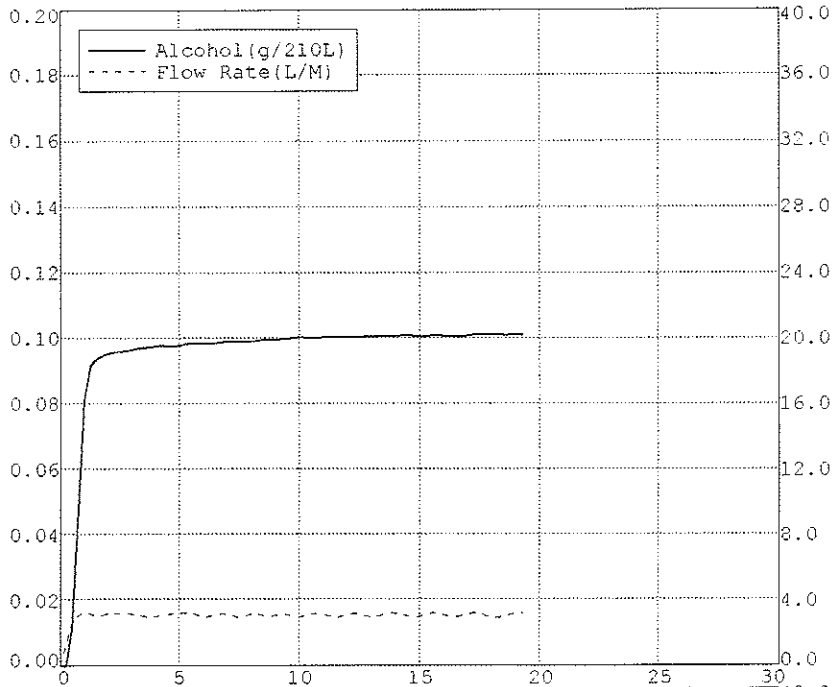

*P. J. 0717*