

SOLUTION CHANGE



WARREN COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 06/02/2023

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 23090

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 14:51 |
| INTERNAL STANDARD | VERIFIED | 14:51 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 14:51 |
| BLANK TEST | 0.00 | 14:52 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.10 | 14:53 |
| BLANK TEST | 0.00 | 14:53 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.10 | 14:54 |
| BLANK TEST | 0.00 | 14:55 |

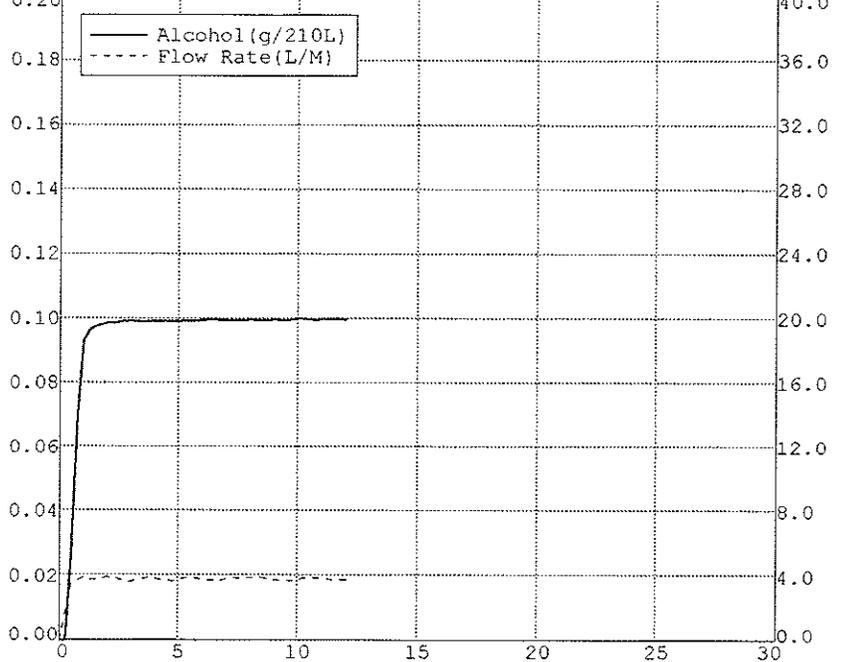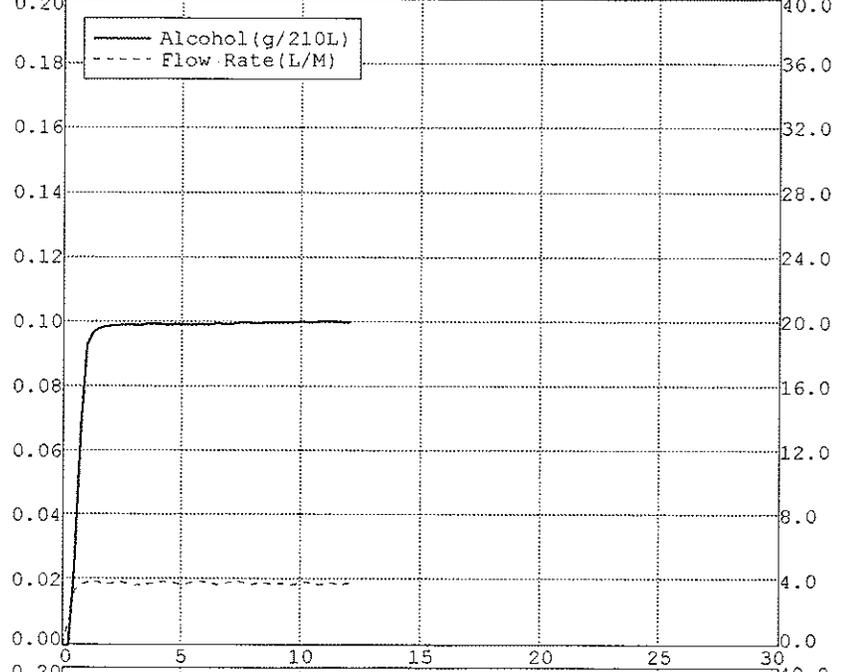

Handwritten signature: C. B. Geisler #241