

SUPERVISOR TEST




WARREN COUNTY  
SHERIFF'S OFFICE  
DATAMASTER dmt: 144506

Date: 06/16/2023

OPERATOR NAME:  
SEAN T SMITH  
Permit #: 46227  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 23090

Nominal = 0.10 g/210L

BLANK TEST	0.00	19:56
INTERNAL STANDARD	VERIFIED	19:56
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	19:57
BLANK TEST	0.00	19:58
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	19:58
BLANK TEST	0.00	19:59
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	19:59
BLANK TEST	0.00	20:00

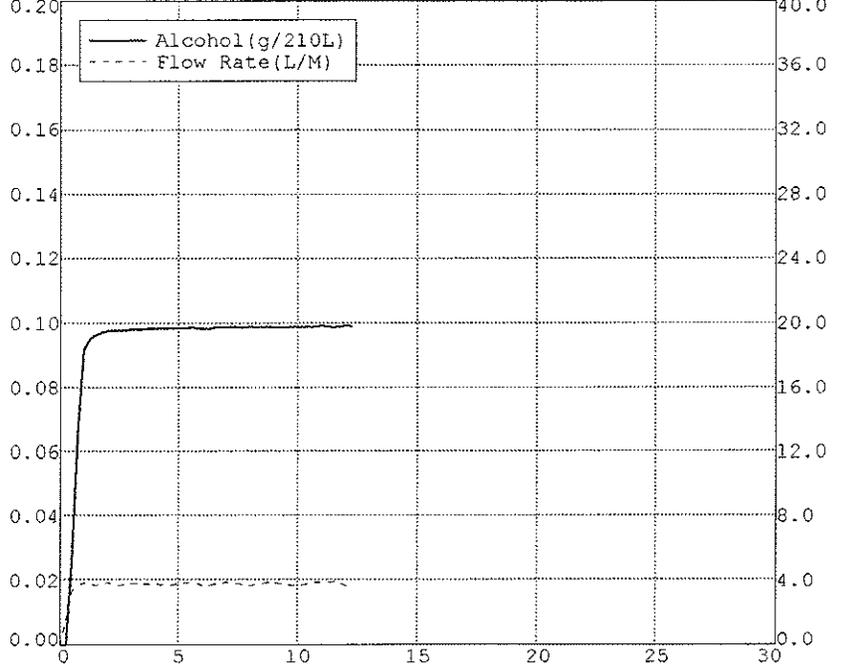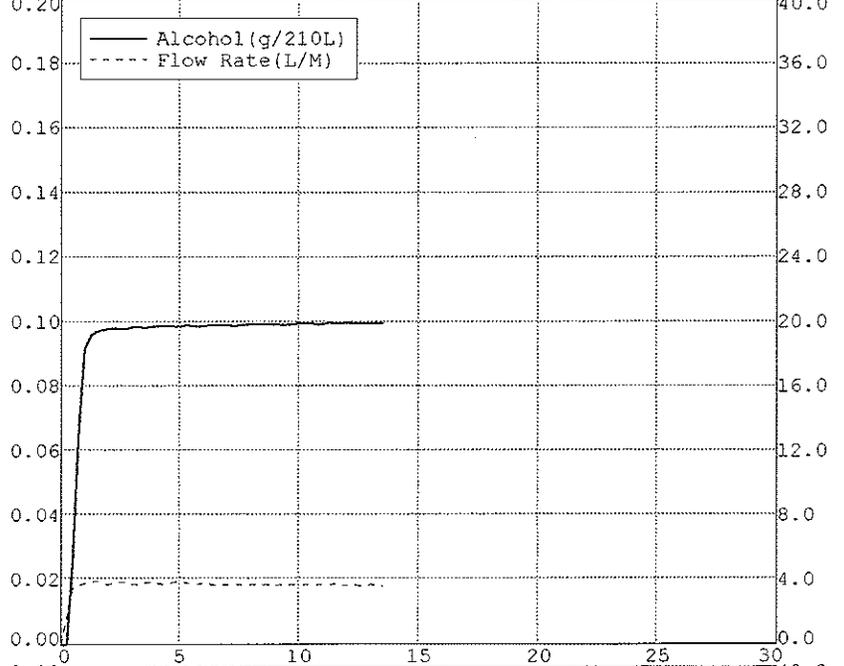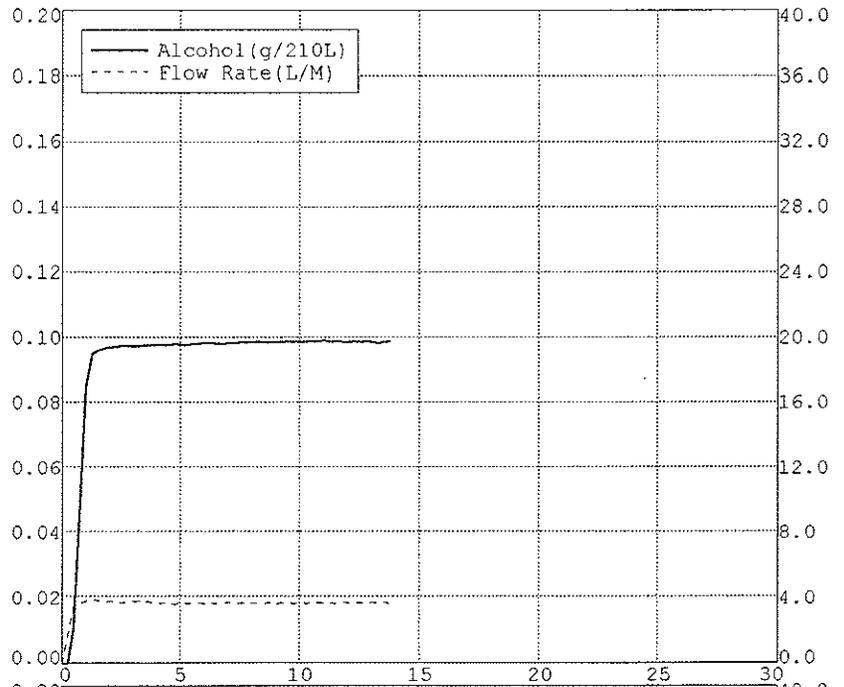

*Handwritten signature and initials*