

SUPERVISOR TEST



WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 03/29/2024

OPERATOR NAME:
MICHAEL A CAMPBELL
Permit #: 42422
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 23430

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:37
INTERNAL STANDARD	VERIFIED	00:37
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:37
BLANK TEST	0.00	00:38
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:38
BLANK TEST	0.00	00:39
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:39
BLANK TEST	0.00	00:40

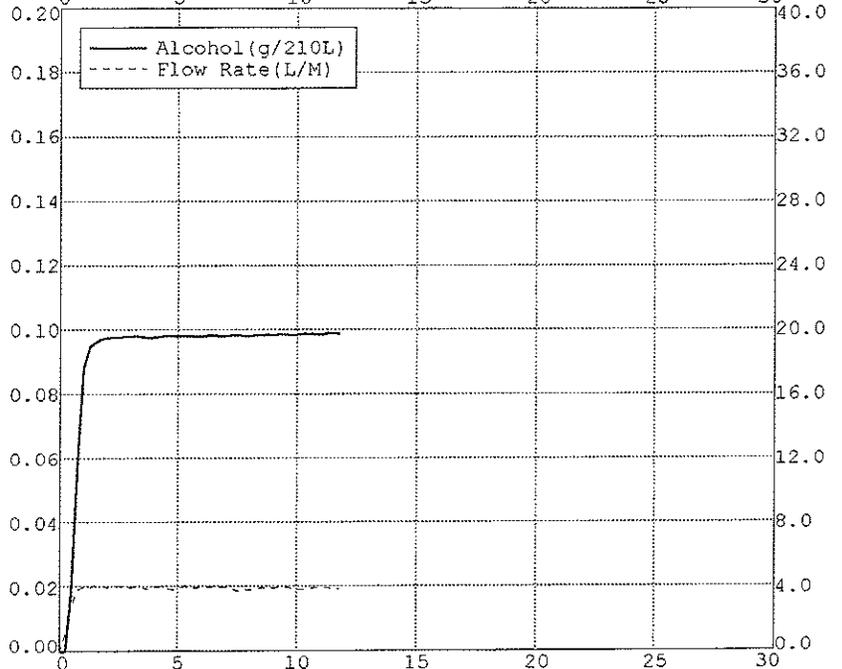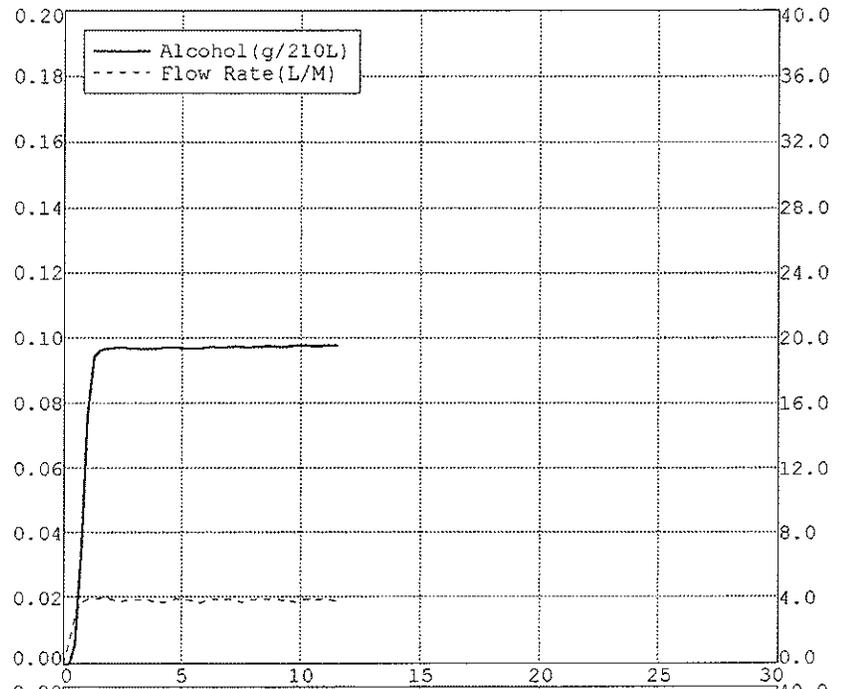

Michael A Campbell #157