

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 06/23/2024

OPERATOR NAME:  
MICHAEL A CAMPBELL  
Permit #: 42422  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 24140

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:09
INTERNAL STANDARD	VERIFIED	00:09
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:10
BLANK TEST	0.00	00:11
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:11
BLANK TEST	0.00	00:12
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:12
BLANK TEST	0.00	00:13

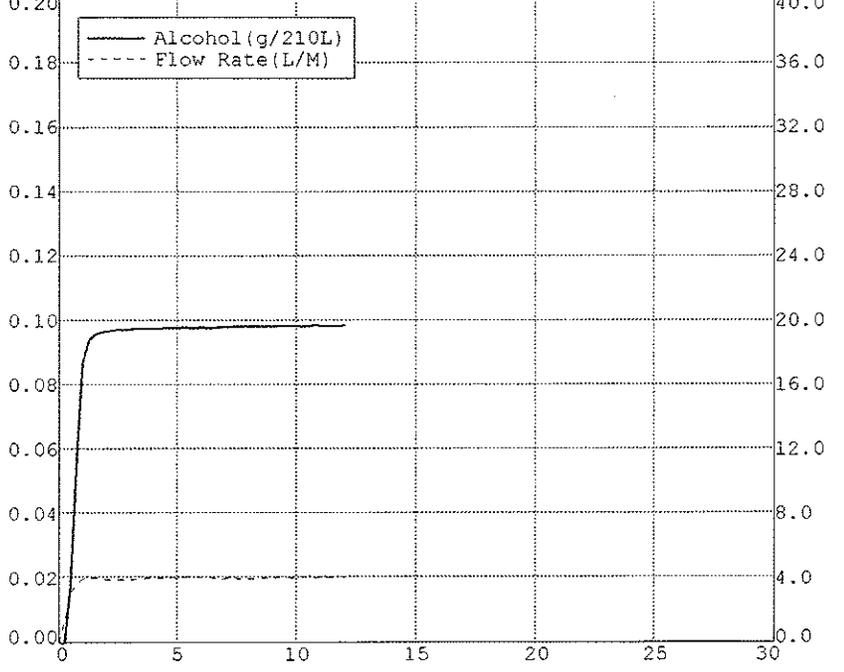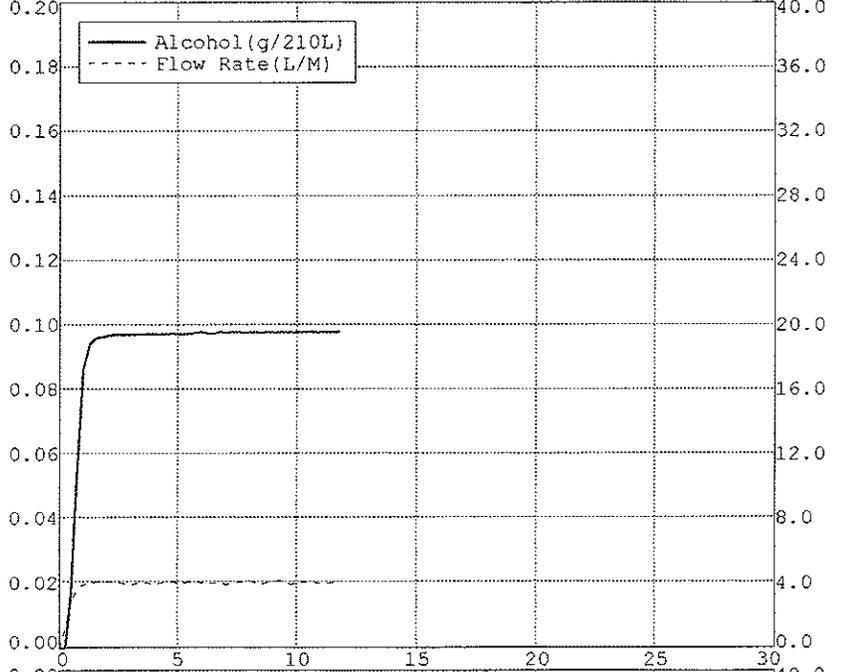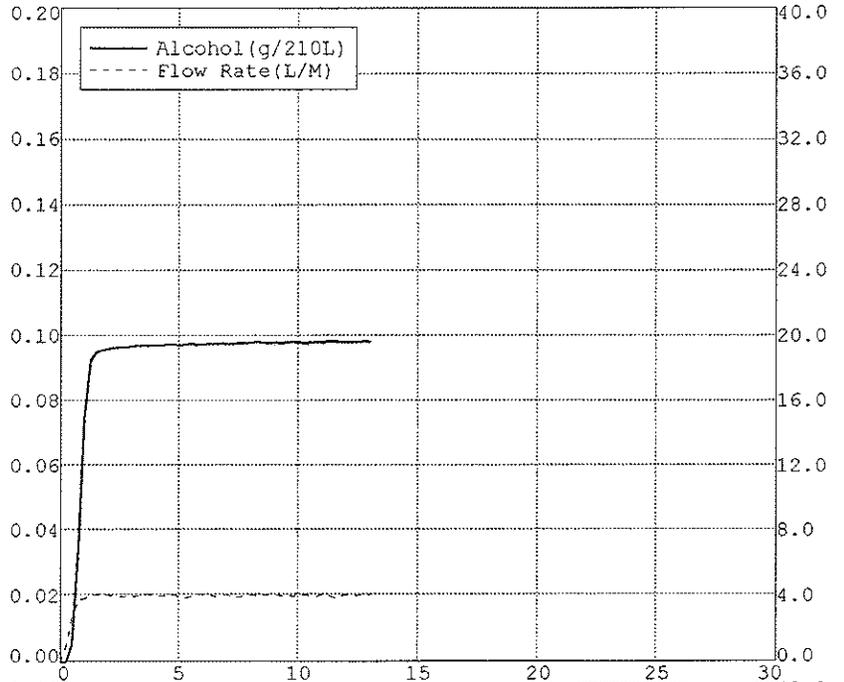

JGT *[Signature]* #157