

SOLUTION CHANGE




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 12/01/2024

OPERATOR NAME:
JOHN D BATEHOLTS
Permit #: 43007
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 24350

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:07
INTERNAL STANDARD	VERIFIED	09:08
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	09:08
BLANK TEST	0.00	09:09
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	09:09
BLANK TEST	0.00	09:10
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	09:10
BLANK TEST	0.00	09:11

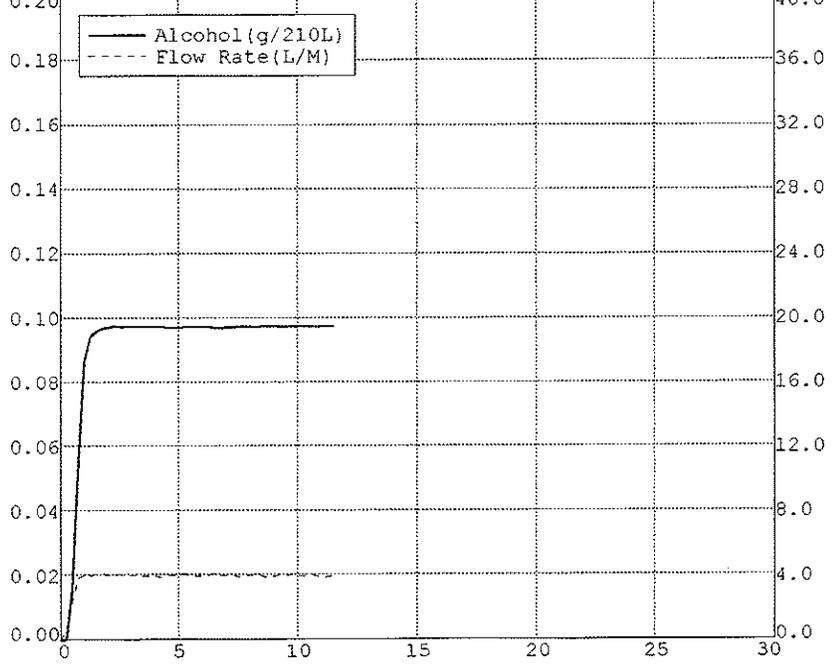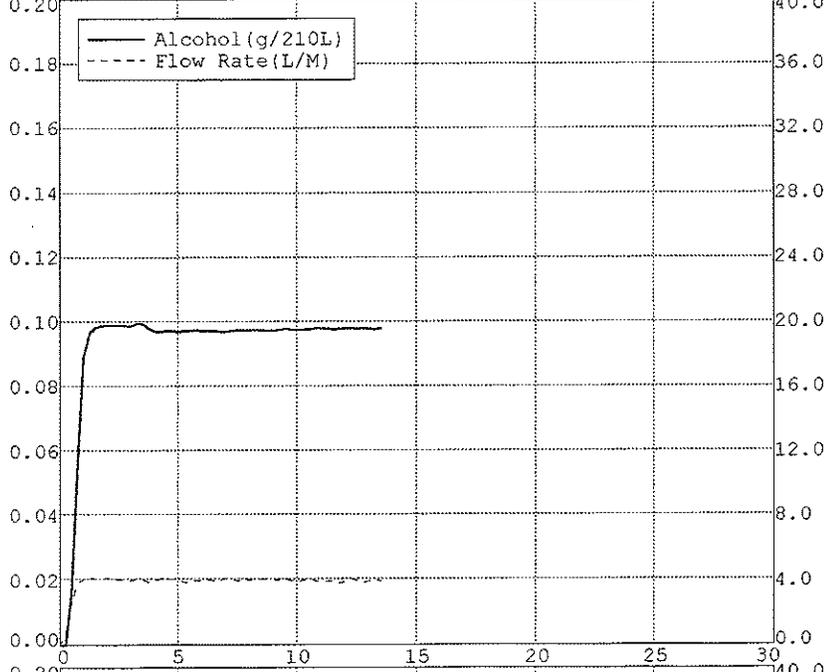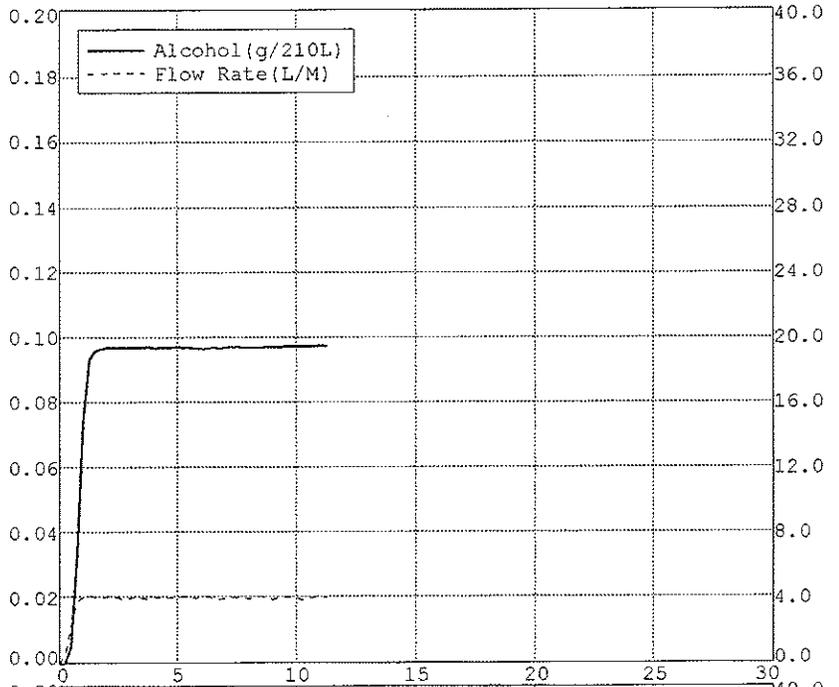

P. [Signature] 07/9