

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 03/29/2024

OPERATOR NAME:  
MICHAEL A CAMPBELL  
Permit #: 42422  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 23430

Nominal = 0.10 g/210L

BLANK TEST	0.00	06:37
INTERNAL STANDARD	VERIFIED	06:37
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	06:38
BLANK TEST	0.00	06:39
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	06:39
BLANK TEST	0.00	06:40
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	06:40
BLANK TEST	0.00	06:41

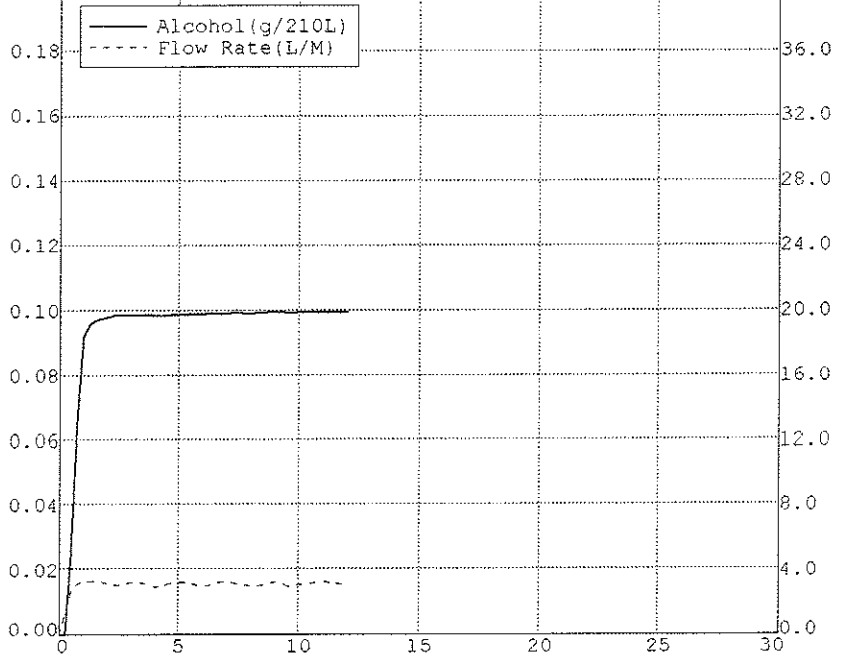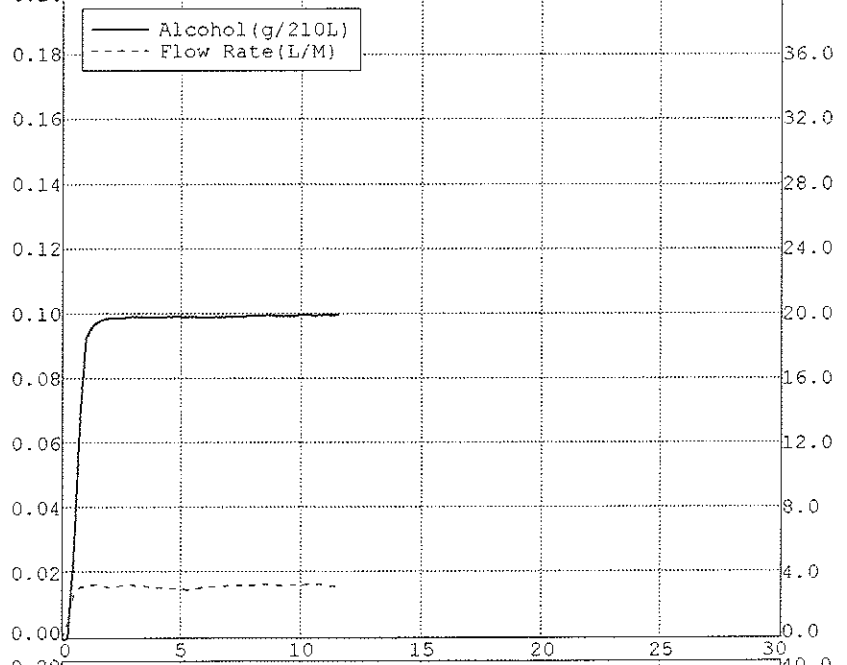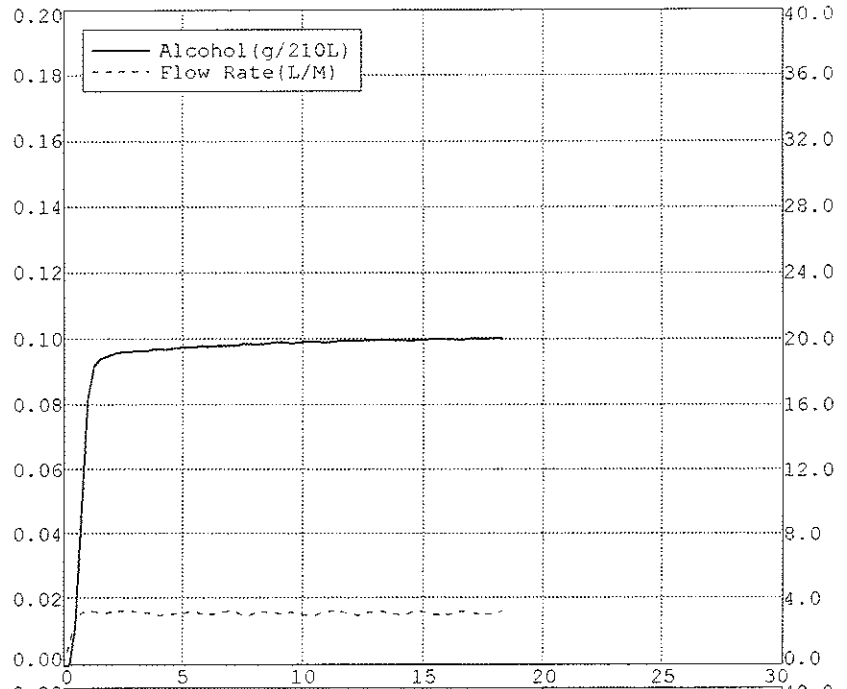

*PO M.A. Campbell #257*